

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133670
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 10 FEB 99
 Serial Number: 139658
 OUIIC: W4GV91

Standards:
 Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: CS-11 Isotope: Cs-137

Calibration:
 Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,080	40,080	1.00	
4k	4010	4010	1.00	
400	400	400	1.00	
100	100	100	1.00	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>16,344</u> dpm	<u>5620</u> (ncpm)	<u>34.39</u>
Beta (2π) <u>25,462</u> dpm	<u>4499</u> (ncpm)	<u>17.67</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 139658.

Date of next calibration: 8 AUG 99

Performed By: Al Perrella

Reviewed By: [Signature]

Report Number: 021099133670

Detector Worksheet

Instrument Model: 2360 Serial Number: 133670

Model: 43-89 Serial Number: 139658

Count time = 60 seconds									
High Voltage	Alpha Source			Beta Source			Background		
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta	
625	3855	429	9.6%	3	1326	0.08%	2	19	
650	4868	343	5.6%	0	2441	0.00%	0	50	
675	5433	331	4.1%	4	3357	0.12%	0	97	
700	5460	360	3.6%	4	4278	0.07%	1	148	
725	5620	502	4.3%	1	4735	0.02%	0	236	
750	5784	1065	7.5%	5	5870	0.09%	0	554	
775	6087	2093	11.7%	3	6773	0.04%	0	1140	

Efficiency Alpha: 34.39% Beta: 17.67%
Background: Alpha : 0 Beta: 236

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133666
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 21 DEC 98
 Serial Number: 139661
 OUIIC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: CS-11 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,155	40,155	1.00	
4k	4,016	4,016	1.00	
400	402	402	1.00	
100	100	100	1.00	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2 π) <u>16,344</u> dpm	<u>6,048</u> (ncpm)	<u>37.31</u>
Beta (2 π) <u>25,414</u> dpm	<u>4,882</u> (ncpm)	<u>19.21</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 139661.

Date of next calibration: 18 JUN 99

Performed By: Al Penella

Reviewed By: Burt Cunningham

Report Number: 122198133666

Detector Worksheet

Instrument Model: 2360 Serial Number: 133666

Model: 43-89 Serial Number: 139661

Count time = 60 seconds								
High Voltage	Alpha Source			Beta Source			Background	
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta
700	5451	355	4.8%	3	3526	0.06%	1	75
725	5851	369	3.8%	3	3909	0.08%	0	135
750	6098	486	3.5%	2	5139	0.04%	0	257
775	6282	858	5.5%	4	6035	0.07%	0	462
800	6493	1221	7.5%	2	6488	0.02%	1	640
825	6368	1971	12.0%	0	7043	0.00%	0	972
850	6354	3000	11.0%	5	8360	0.04%	2	1971

Efficiency Alpha: 37.31% Beta: 19.21%

Background: Alpha : 0 Beta: 257

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133661
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 21 DEC 98
 Serial Number: 139117
 OUC: W4GV91

Standards:
 Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: CS-11 Isotope: Cs-137

Calibration:
 Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,187	40,187	1.00	
4k	4,019	4,019	1.00	
400	402	402	1.00	
100	100	100	1.00	
40	41	41	.98	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>16,344</u> dpm	<u>6,320</u> (ncpm)	<u>38.67</u>
Beta (2π) <u>25,414</u> dpm	<u>5,053</u> (ncpm)	<u>19.88</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 139117.

Date of next calibration: 18 JUN 99

Performed By: Al Penella

Reviewed By: Bruce [Signature]

Report Number: 122198133661

Detector Worksheet

Instrument Model: 2360 Serial Number: 133661

Model: 43-89 Serial Number: 139117

Count time = 60 seconds								
High Voltage	Alpha Source			Beta Source			Background	
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta
550	5202	327	4.9%	4	2810	0.11%	1	55
575	5880	371	4.2%	4	3983	0.10%	0	106
600	6320	421	3.2%	3	5259	0.06%	0	206
625	6445	911	6.6%	2	5939	0.03%	0	423
650	6376	2420	18.2%	7	6966	0.10%	0	821
675	6575	4496	26.8%	4	7909	0.05%	0	1532

Efficiency Alpha: 38.67% Beta: 19.88%

Background: Alpha : 0 Beta: 206

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133670
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 20 NOV 98
 Serial Number: 139658
 OUC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 04 DEC 98
 Calibration Due: 04 DEC 98
 Source: CS-11 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,098	40,098	1.00	
4k	4010	4010	1.00	
400	401	401	1.00	
100	100	100	1.00	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) 16,344 dpm	6016 (ncpm)	36.81
Beta (2π) 25,462 dpm	4823 (ncpm)	18.94

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 139658. DATE of next calibrations: 18 May 99.

Performed By: Al Penella

Reviewed By: [Signature]

Report Number: 112098133670

Detector Worksheet

Instrument Model: 2360 Serial Number: 133670

Model: 43-89 Serial Number: 139658

Count time = 60 seconds								
High Voltage	Alpha Source			Beta Source			Background	
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta
575	2842	533	15.1%	2	939	0.21%	0	24
600	4191	394	7.7%	1	1770	0.00%	1	40
625	4931	368	5.7%	4	2876	0.14%	0	65
650	5577	463	5.2%	5	4040	0.12%	0	150
675	6016	693	6.1%	2	5109	0.04%	0	286
700	6226	1038	5.4%	7	5827	0.12%	0	643
725	6087	1995	9.5%	3	7222	0.03%	1	1224

Efficiency Alpha: 36.81% Beta: 18.94%
Background: Alpha : 0 Beta: 286

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 141308
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 20 NOV 98
 Serial Number: 139659
 OUC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 04 DEC 98
 Calibration Due: 04 DEC 98
 Source: CS-11 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	39,959	39,959	1.00	
4k	3996	3996	1.00	
400	400	400	1.00	
100	99	99	1.01	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) 16,344 dpm	6386 (ncpm)	39.07
Beta (2π) 25,462 dpm	4795 (ncpm)	18.83

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 139659. DATE of NEXT CALIBRATION: 18 MAY 99.

Performed By: Al Perrella

Reviewed By: [Signature]

Report Number: 112098141308

Detector Worksheet

Instrument Model: 2360 Serial Number: 141308

Model: 43-89 Serial Number: 139659

Count time = 60 seconds								
High Voltage	Alpha Source			Beta Source			Background	
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta
550	2290	542	18.4%	1	780	0.13%	0	22
575	4593	509	9.2%	0	1789	0.00%	0	38
600	5562	400	5.7%	2	2939	0.07%	0	62
625	6179	446	4.8%	3	4046	0.07%	0	131
650	6386	465	3.1%	2	5048	0.04%	0	253
675	6431	1345	5.6%	5	5660	0.09%	0	907
700	6630	2040	7.8%	5	6100	0.08%	0	1360

Efficiency **Alpha: 39.07%** **Beta: 18.83%**
Background: **Alpha :** **0** **Beta:** **253**

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133668
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 20 NOV 98
 Serial Number: 136345
 OUC: W4GV91

Standards:
 Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 04 DEC 98
 Calibration Due: 04 DEC 98
 Source: CS-11 Isotope: Cs-137

Calibration:
 Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	39,930	39,930	1.00	
4k	3993	3993	1.00	
400	399	399	1.00	
100	100	100	1.00	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>16,344</u> dpm	<u>5969</u> (ncpm)	<u>36.52</u>
Beta (2π) <u>25,462</u> dpm	<u>4497</u> (ncpm)	<u>17.66</u>

Remarks:
 This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 136345. DATE of next calibration: 18 MAY 99.

Performed By: Al Perrella

Reviewed By: [Signature]

Report Number: 112098/133668

Detector Worksheet

Instrument Model: 2360 Serial Number: 133668

Model: 43-89 Serial Number: 136345

Count time = 60 seconds									
High Voltage	Alpha Source			Beta Source			Background		
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta	
625	2042	583	21.3%	0	500	0.00%	0	23	
650	3610	444	10.1%	1	1268	0.08%	0	34	
675	4701	362	6.3%	3	1985	0.15%	0	43	
700	5642	339	4.4%	4	3027	0.10%	1	76	
725	5821	355	3.9%	4	3788	0.11%	0	116	
750	5969	510	3.5%	3	4782	0.06%	0	285	
775	6092	1041	3.0%	6	5894	0.10%	0	824	

Efficiency Alpha: 36.52% Beta: 17.66%
Background: Alpha : 0 Beta: 285

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133661
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 3 JUN 99
 Serial Number: 139117
 OUC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: CS-11 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,090	40,090	1.00	
4k	4,010	4,010	1.00	
400	401	401	1.00	
100	100	100	1.00	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>16,344</u> dpm	<u>6192</u> (ncpm)	<u>37.89</u>
Beta (2π) <u>25,151</u> dpm	<u>5100</u> (ncpm)	<u>20.28</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. As found readings were within specifications. No high voltage plateau performed. Calibrated with Probe SN: 139117.

Date of next calibration: 29 NOV 99

Performed By: M Penelle

Reviewed By: Burt [Signature]

Report Number: 060399133661

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133666
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 3 JUN 99
 Serial Number: 139661
 OUC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: CS-11 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,145	40,145	1.00	
4k	4,009	4,009	1.00	
400	402	402	1.00	
100	100	100	1.00	
40	41	41	.98	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>16,344</u> dpm	<u>6216</u> (ncpm)	<u>38.03</u>
Beta (2π) <u>25,151</u> dpm	<u>4725</u> (ncpm)	<u>18.79</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. As found readings were within specifications. No high voltage plateau performed. Calibrated with Probe SN: 139661.

Date of next calibration: 29 NOV 99

Performed By: al Penelle

Reviewed By: [Signature]

Report Number: 060399/133666

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 141308
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 14 MAY 99
 Serial Number: 139659
 OUC: W4GV91

Standards:
 Pulser Serial Number: 43859 Calibration Due: 25 NOV 99
 Volt/Ohm Meter Serial Number: 43859 Calibration Due: 25 NOV 99
 Source: P-420 Isotope: Pu-239 Source: CS-11 Isotope: Cs-137

Calibration:
 Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	1K	1.00
x100	1k	1K	400	1.00
x10	400	400	100	1.00
x10	100	100	400 100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	39,970	39,970	1.00	
4k	3,997	3,997	1.00	
400	402	402	1.00	
100	101	101	.99	
40	41	41	.98	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>16,344</u> dpm	<u>6100</u> (ncpm)	<u>37.32</u>
Beta (2π) <u>25,183</u> dpm	<u>4782</u> (ncpm)	<u>18.99</u>

Remarks:
 This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 139659. ASEVND Readings were within specifications. No high voltage plateau performed.

Date of next calibration: 9 NOV 99.

Performed By: Al Perrella

Reviewed By: [Signature]

Report Number: 051499141308

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133668
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 14 MAY 99
 Serial Number: 136345
 OUC: W4GV91

Standards:

Pulsar Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: CS-11 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,110	40,110	1.00	
4k	4,008	4,008	1.00	
400	401	401	1.00	
100	99	99	1.01	
40	41	41	.98	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>16,344</u> dpm	<u>5882</u> (ncpm)	<u>35.99</u>
Beta (2π) <u>25,183</u> dpm	<u>4350</u> (ncpm)	<u>17.27</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 136345. As FOUND Readings were within specifications. No high voltage plateau performed.

Date of next calibration: 9 NOV 99.

Performed By: al Penella

Reviewed By: Bert Hummer

Report Number: 051499136345

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133670
 Detector Model: 43-89
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 17 JUN 99
 Serial Number: 139658
 OUC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: P-420 Isotope: Pu-239

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: CS-11 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	0	40K	1.00
x1000	10k	0	10K	1.00
x100	4k	0	4K	1.00
x100	1k	0	1K	1.00
x10	400	0	400	1.00
x10	100	0	100	1.00
x1	40	0	40	1.00
x1	10	0	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	0	40312	.99	
4k	0	4026	.99	
400	0	403	.99	
100	0	100	1.00	
40	0	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>16,344</u> dpm	<u>6017</u> (ncpm)	<u>36.81</u>
Beta (2π) <u>25,259</u> dpm	<u>4738</u> (ncpm)	<u>18.76</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. *Replaced photo-multiplier tube in detector model number 43-89, serial number 139658. Calibrated with Probe SN: 139658.

Date of next calibration: 13 DEC 99.

Performed By: Al Perrella

Reviewed By: Burt Cummings

Report Number: 061799133670

Detector Worksheet

Instrument Model: 2360 Serial Number: 133670

Model: 43-89 Serial Number: 139658

High Voltage	Alpha Source			Beta Source			Background	
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta
525	4158	392	7.6%	3	1553	0.13%	1	47
550	5142	337	4.9%	6	2969	0.20%	0	67
575	5658	385	4.2%	5	4120	0.10%	1	129
600	6017	624	6.2%	3	4952	0.06%	0	214
625	6177	1484	13.9%	6	5886	0.10%	0	418
650	6069	5026	35.1%	2	7443	0.03%	0	1135

Efficiency Alpha: 36.81% Beta: 18.76%

Background: Alpha : 0 Beta: 214

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 133663
 Detector Model: 43-37-1
 Detector Type: GAS FLOW PROPORTIONAL
 Type Of Calibration: Electronic/Source

Date: 23 Nov 98
 Serial Number: 136362
 OUIIC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: ES927 Isotope: Pu-238

Calibration Due: 04 DEC 98
 Calibration Due: 04 DEC 98
 Source: H-045 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,048	40,048	1.00	
4k	4,004	4,004	1.00	
400	401	401	1.00	
100	100	100	1.00	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>15,900</u> dpm	<u>3761</u> (ncpm)	<u>23.65</u>
Beta (2π) <u>82,008</u> dpm	<u>33013</u> (ncpm)	<u>40.26</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 136362. DATE OF NEXT CALIBRATION: 21 MAY 99

Performed By: Al Penick

Reviewed By: Bud Hummer

Report Number: 112398133663

Detector Worksheet

Instrument Model: 2360 Serial Number: 133663

Model: 43-37-1 Serial Number: 136362

High Voltage	Alpha Source			Beta Source			Background	
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta
1700	2668	883	11.5%	2	30355	0.00%	2	476
1725	2718	824	8.9%	3	31815	0.00%	2	510
1750	3241	1207	8.6%	2	35408	0.00%	1	825
1775	3764	1399	7.3%	38	34037	0.10%	3	1024
1800	4212	1424	5.7%	172	31691	0.52%	6	1104
1825	4584	1531	7.2%	505	28691	1.69%	12	1092

Efficiency: **Alpha: 23.65%** **Beta: 40.26%**
Background: **Alpha: 3 cpm** **Beta: 1024 cpm**

Ludlum Model 2224-1 Calibration Data Sheet

Serial Number: 129468
 Detector Model: 43-37-1
 Detector Type: GAS FLOW PROPORTIONAL
 Type Of Calibration: Electronic/Source

Date: 30 NOV 98
 Serial Number: 136363
 OUC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: ES927 Isotope: Pu-238

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: H-045 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40192	40192	1.00	
4k	4018	4018	1.00	
400	402	402	1.01	
100	100	100	1.00	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) 15,897 dpm	4241 (ncpm)	26.68
Beta (2π) 81,973 dpm	32203 (ncpm)	39.28

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 136363. DATE OF NEXT CALIBRATION: 28 MAY 99.

Performed By: Al Perrella

Reviewed By: Burt Hummer

Report Number: 113098129468

Detector Worksheet

Instrument Model: 2224-1 Serial Number: 129468

Model: 43-37-1 Serial Number: 136363

Count time = 60 seconds									
High Voltage	Alpha Source			Beta Source			Background		
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta	
1650	2463	711	12.7%	1	26234	0.00%	1	308	
1675	2914	799	8.7%	3	30414	0.00%	4	477	
1700	3224	933	9.0%	4	33696	0.00%	3	557	
1725	3636	1098	7.1%	1	35251	0.00%	1	763	
1750	4040	1328	6.9%	8	35047	0.01%	5	956	
1775	4243	1398	6.4%	53	33239	0.15%	2	1036	
1800	4746	1398	6.0%	335	29779	1.10%	4	1030	
1825	5082	1319	3.8%	1006	25189	3.80%	11	1076	

Efficiency Alpha: 26.68% Beta: 39.28%

Background: Alpha : 2 Beta: 1036

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 141313
 Detector Model: 43-37-1
 Detector Type: GAS FLOW PROPORTIONAL
 Type Of Calibration: Electronic/Source

Date: 23 Nov 98
 Serial Number: 145076
 OUC: W4GV91

Standards:

Pulsar Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: ES927 Isotope: Pu-238

Calibration Due: 04 DEC 98
 Calibration Due: 04 DEC 98
 Source: H-045 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00

Digital Readout (Integrate/Scaler Mode)			
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
40k	40,039	40,039	1.00
4k	4003	4003	1.00
400	401	401	1.00
100	99	99	1.01
40	40	40	1.00

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>15,900</u> dpm	<u>3625</u> (ncpm)	<u>22.80</u>
Beta (2π) <u>82,008</u> dpm	<u>33375</u> (ncpm)	<u>40.70</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 145076. DATE of NEXT CALIBRATION: ~~18 May 99~~
21 May 99.

Performed By: Al Penella

Reviewed By: Bud [Signature]

Report Number: 112398141313

Detector Worksheet

Instrument Model: 2360 Serial Number: 141313
Model: 43-37-1 Serial Number: 145076

High Voltage	Alpha Source			Beta Source			Background	
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta
1725	2230	980	12.3%	1	32677	-0.01%	3	585
1750	2854	1160	7.4%	0	36497	-0.01%	5	862
1775	3278	1382	7.9%	8	36161	0.02%	2	1013
1800	3628	1550	8.8%	55	34467	0.15%	3	1092
1825	4089	1523	7.2%	208	31740	0.64%	4	1117
1850	4427	1544	8.3%	1011	26778	3.56%	21	1046

Efficiency: Alpha: 22.80%
Background: Alpha: 3 cpm

Beta: 40.70%
Beta: 1092 cpm

Ludlum Model 2224-1 Calibration Data Sheet

Serial Number: 129447
 Detector Model: 43-37-1
 Detector Type: GAS FLOW PROPORTIONAL
 Type Of Calibration: Electronic/Source

Date: 30 NOV 98
 Serial Number: 134334
 OUIIC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: ES927 Isotope: Pu-238

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: H-045 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40430	40430	1.01	
4k	4002	4002	1.00	
400	402	402	1.01	
100	100	100	1.00	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) 15,897 dpm	4615 (ncpm)	29.03
Beta (2π) 81,973 dpm	33616 (ncpm)	41.01

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 134334. DATE OF NEXT CALIBRATION: 28 MAY 99.

Performed By: Al Penella

Reviewed By: [Signature]

Report Number: 113098129447

Detector Worksheet

Instrument Model: 2224-1 Serial Number: 129447

Model: 43-37-1 Serial Number: 134334

Count time = 60 seconds									
High Voltage	Alpha Source			Beta Source			Background		
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta	
1625	2597	621	10.4%	3	24020	0.01%	1	286	
1650	2942	802	10.9%	1	27547	-0.01%	4	395	
1675	3219	839	9.0%	3	30904	0.01%	1	474	
1700	3772	1008	7.5%	2	34025	0.00%	2	651	
1725	4062	1178	7.0%	6	35473	0.01%	3	812	
1750	4620	1333	6.7%	27	34551	0.06%	5	935	
1775	4950	1436	6.3%	196	31608	0.60%	5	1036	

Efficiency Alpha: 29.03% Beta: 41.01%
Background: Alpha : 5 Beta: 935

Ludlum Model 2224-1 Calibration Data Sheet

Serial Number: 129447
 Detector Model: 43-37-1
 Detector Type: GAS FLOW PROPORTIONAL
 Type Of Calibration: Electronic/Source

Date: 19 APR 99
 Serial Number: 134334
 OUIIC: W4GV91

Standards:

Pulsar Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: ES927 Isotope: Pu-238

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: H-045 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40K	40200	40200	1.00	
4k	4001	4001	1.00	
400	401	401	1.00	
100	100	100	1.00	
40	40	40	1.00	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>15,849</u> dpm	<u>4,586</u> (ncpm)	<u>28.94</u>
Beta (2π) <u>81,275</u> dpm	<u>32,295</u> (ncpm)	<u>39.74</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. Calibrated with Probe SN: 134334. DATE OF NEXT CALIBRATION: 15 OCT 99.

Performed By: Al Penella

Reviewed By: Burt Linneman

Report Number: 041999129447

Detector Worksheet

Instrument Model: 2224-1 Serial Number: 129447

Model: 43-37-1 Serial Number: 134334

Count time = 60 seconds									
High Voltage	Alpha Source			Beta Source			Background		
	Alpha	Beta	xtalk	Alpha	Beta	xtalk	Alpha	Beta	
1600	2437	667	13.2%	1	23221	0.00%	1	257	
1625	2951	744	9.8%	1	28020	-0.01%	5	383	
1650	3433	949	10.5%	3	33305	0.00%	2	488	
1675	3889	1056	8.0%	2	35255	-0.01%	4	661	
1700	4313	1253	7.1%	10	35270	0.01%	8	857	
1725	4591	1412	7.1%	68	33282	0.19%	5	987	
1750	4883	1479	6.3%	339	30038	1.09%	7	1077	

Efficiency Alpha: 28.94% Beta: 39.74%

Background: Alpha : 5 Beta: 987

Ludlum Model 2360 Calibration Data Sheet

Serial Number: 141313
 Detector Model: 43-37-1
 Detector Type: SCINTILLATION
 Type Of Calibration: Electronic/Source

Date: 15 JUN 99
 Serial Number: 145076
 OUIC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: ES927 Isotope: Pu-238

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: H-045 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40k	40k	1.00
x1000	10k	10k	10k	1.00
x100	4k	4k	4k	1.00
x100	1k	1k	1k	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,051	40,051	1.00	
4k	4,011	4,011	1.00	
400	401	401	1.00	
100	100	100	1.00	
40	41	41	.98	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) 15,829 dpm	3789 (ncpm)	23.94
Beta (2π) 80,961 dpm	33209 (ncpm)	41.02

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. As found readings were within specifications. No high voltage plateau performed. Calibrated with Probe SN: 145076.

Date of next calibration: 11 DEC 99.

Performed By: Al Perrella

Reviewed By: [Signature]

Report Number: 061599145076

Ludlum Model 2224-1 Calibration Data Sheet

Serial Number: 129468
 Detector Model: 43-37-1
 Detector Type: GAS FLOW PROPORTIONAL
 Type Of Calibration: Electronic/Source

Date: 15 JUN 99
 Serial Number: 136363
 OUC: W4GV91

Standards:

Pulser Serial Number: 43859
 Volt/Ohm Meter Serial Number: 43859
 Source: ES927 Isotope: Pu-238

Calibration Due: 25 NOV 99
 Calibration Due: 25 NOV 99
 Source: H-045 Isotope: Cs-137

Calibration:

Beta Threshold: 3.5 mV Beta Window: 30 mV Alpha Threshold: 120 mV

Rate Meter				
Meter Range	Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor
x1000	40k	40K	40K	1.00
x1000	10k	10K	10K	1.00
x100	4k	4K	4K	1.00
x100	1k	1K	1K	1.00
x10	400	400	400	1.00
x10	100	100	100	1.00
x1	40	40	40	1.00
x1	10	10	10	1.00
Digital Readout (Integrate/Scaler Mode)				
Applied (cpm)	Initial Reading (cpm)	Final Reading (cpm)	Correction Factor	
40k	40,210	40,210	.99	
4k	4,081	4,081	.98	
400	402	402	1.00	
100	101	101	.99	
40	41	41	.98	

Source Activity	Meter Indication	Efficiency (%)
Alpha (2π) <u>15,829</u> dpm	4540 <u>4484</u> (ncpm)	<u>28.33</u>
Beta (2π) <u>80,961</u> dpm	<u>30169</u> (ncpm)	<u>37.26</u>

Remarks:

This calibration is Traceable to the National Institute of Standards and Technology. Set up Response Test Range Prior to initial use. As found readings were within specifications. No high voltage plateau performed. Calibrated with Probe SN: 136363.

Date of next calibration: 11 DEC 99

Performed By: Al Perrella

Reviewed By: [Signature]

Report Number: 061599129468

EBERLINE SPA-8 CALIBRATION REPORT

Date: 11/28/98
Standard: Model 81
SN: 7140

OUI: W4GV91
Isotope: Cs-137
Type of Calibration: Source

E-600 Serial Number	926
Program Version	E600 V3.09
Calibration Date	12/30/97
Calibration Due Date	12/30/99
Scaler Precision	10%
Lower Threshold Slope	0.9048
Lower Threshold Intercept	-0.0857 mV
Upper Threshold Slope	1.08
Upper Threshold Intercept	-0.5926 mV
Alarm Editing	Enabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	723416
Type	SPA-8
Calibration Date	11/28/98
Calibration Due Date	05/26/99
Dead Time	12.0 usec
Surface Area	5.00 cm ²
Max High Voltage	1500 Vdc
Overrange	45000 cps

Channel 1	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	10 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 2	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	10 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 3	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	10 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0

Gamma Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
0.0040 R/hr	0.0041 R/hr	3.30%	Pass
0.0004 R/hr	0.0004 R/hr	9.69%	Pass
1.00E-04 R/hr	0.0001 R/hr	8.7%	Pass
4.00E-05 R/hr	3.67E-05 R/hr	8.31%	Pass

Response Test Range: 11.24 - 16.86 μ R/hr (BKG CORRECTED)

Remarks:

This calibration is traceable to the National Institute of Standards and Technology.

Response tested with Cs-137, SN: CS-99R. As found data: 0.0045, 0.00047, 0.0001, and 0.00004 R/hr respectively.

Date of next calibration: 26 MAY 99.


Performed By: Al Perrella

Reviewed By: [Signature]

Report number: 112898723416

SPA-8 723416 Voltage Plateau Curve

C
o
u
n
t
s
/
S
e
c

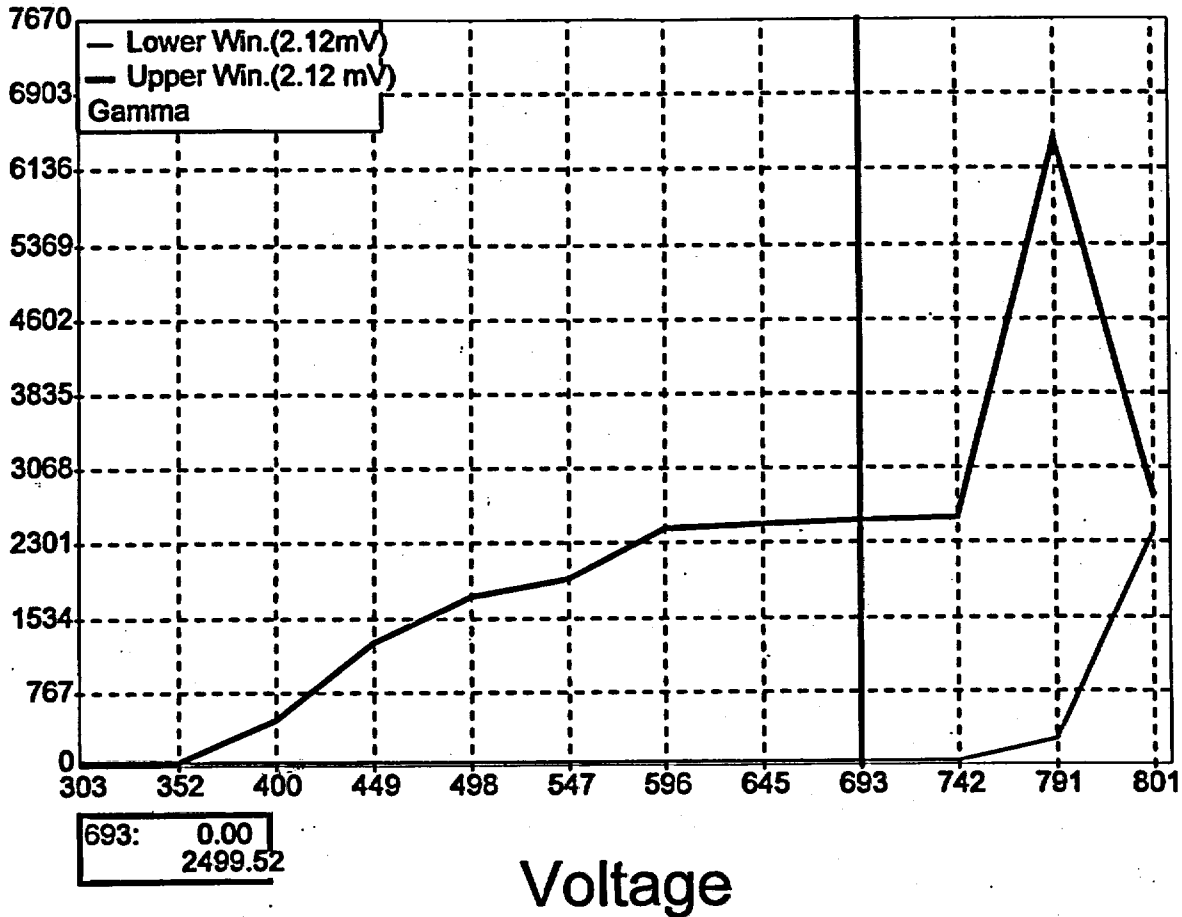

EBERLINE SPA-8 CALIBRATION REPORT

Date: 11/12/98
Standard: Model 81
SN: 7140

OUIC: W4GV91
Isotope: Cs-137
Type of Calibration: Source

E-600 Serial Number	921
Program Version	E600 V3.09
Calibration Date	02/17/98
Calibration Due Date	02/17/99
Scaler Precision	10%
Lower Threshold Slope	0.9048
Lower Threshold Intercept	-0.1524 mV
Upper Threshold Slope	0.9222
Upper Threshold Intercept	-0.7556 mV
Alarm Editing	Disabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Enabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	723413
Type	S-SPA-8
Calibration Date	11/12/98
Calibration Due Date	05/10/99
Dead Time	18.0 usec
Surface Area	5.00 cm²
Max High Voltage	1500 Vdc
Overrange	45000 cps

Channel 1	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	120 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 2	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	120 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 3	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	120 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0

Gamma Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
0.0040 R/hr	0.0042 R/hr	4.73%	Pass
0.0004 R/hr	0.0004 R/hr	2.34%	Pass
1.00E-04 R/hr	9.22E-05 R/hr	-7.82%	Pass
4.00E-05 R/hr	4.14E-05 R/hr	3.47%	Pass

Response Test Range: 11.84 - 17.76 μ R/hr (BKT CORRECTED)

Remarks:

This calibration is traceable to the National Institute of Standards and Technology.

Response tested with Cs-137, SN: CS-99R. As found data: 0.0042, 0.00043, 0.00011, and 0.000043 R/hr respectively.

Date of next calibration: 10 MAY 99.


Performed By: Ol Penella

Reviewed By: Bert [Signature]

Report number: 111298723413

SPA-8 723413 Voltage Plateau Curve

C
o
u
n
t
s
/
s
e
c

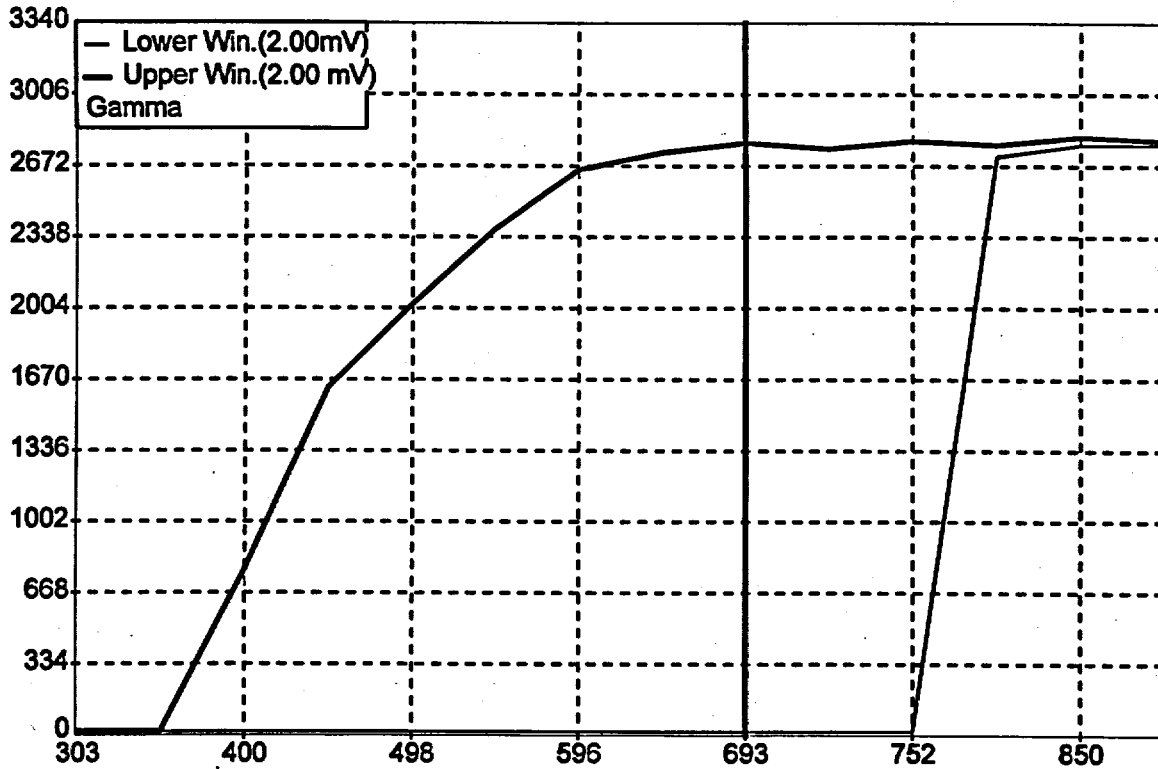

693:	0.00
	2758.69

Voltage

EBERLINE SPA-8 CALIBRATION REPORT

Date: 11/12/98
Standard: Model 81
SN: 7140

OUIIC: W4GV91
Isotope: Cs-137
Type of Calibration: Source

E-600 Serial Number	926
Program Version	E600 V3.09
Calibration Date	11/12/97
Calibration Due Date	12/11/98
Scaler Precision	10%
Lower Threshold Slope	0.9048
Lower Threshold Intercept	-0.0857 mV
Upper Threshold Slope	1.08
Upper Threshold Intercept	-0.5926 mV
Alarm Editing	Enabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	724038
Type	SSPA-8
Calibration Date	11/12/98
Calibration Due Date	05/10/99
Dead Time	15.5 usec
Surface Area	5.00 cm ²
Max High Voltage	1500 Vdc
Overrange	45000 cps

Channel 1	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	645 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.06E+10 counts/R
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 2	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	645 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.06E+10 counts/R
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 3	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	645 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.06E+10 counts/R
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0

Gamma Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
0.0040 R/hr	0.0041 R/hr	2.61%	Pass
0.0004 R/hr	0.0004 R/hr	0.6698%	Pass
1.00E-04 R/hr	9.18E-05 R/hr	-8.19%	Pass
4.00E-05 R/hr	4.25E-05 R/hr	0.35%	Pass

Response Test Range: 7.13 - 10.69 μ R/hr (BKG CORRECTED)

Remarks:

This calibration is traceable to the National Institute of Standards and Technology.

Response tested with Cs-137, SN: CS-99R. As found data: 0.0043, 0.00042, 0.00011, and 0.000043 R/hr respectively.

Date of next calibration: 10 MAY 99.


Performed By: Al Perrella

Reviewed By: Burt Hummer

Report number: 111298724038

SPA-8 724038 Voltage Plateau Curve

C
O
U
N
T
S
/
S
E
C

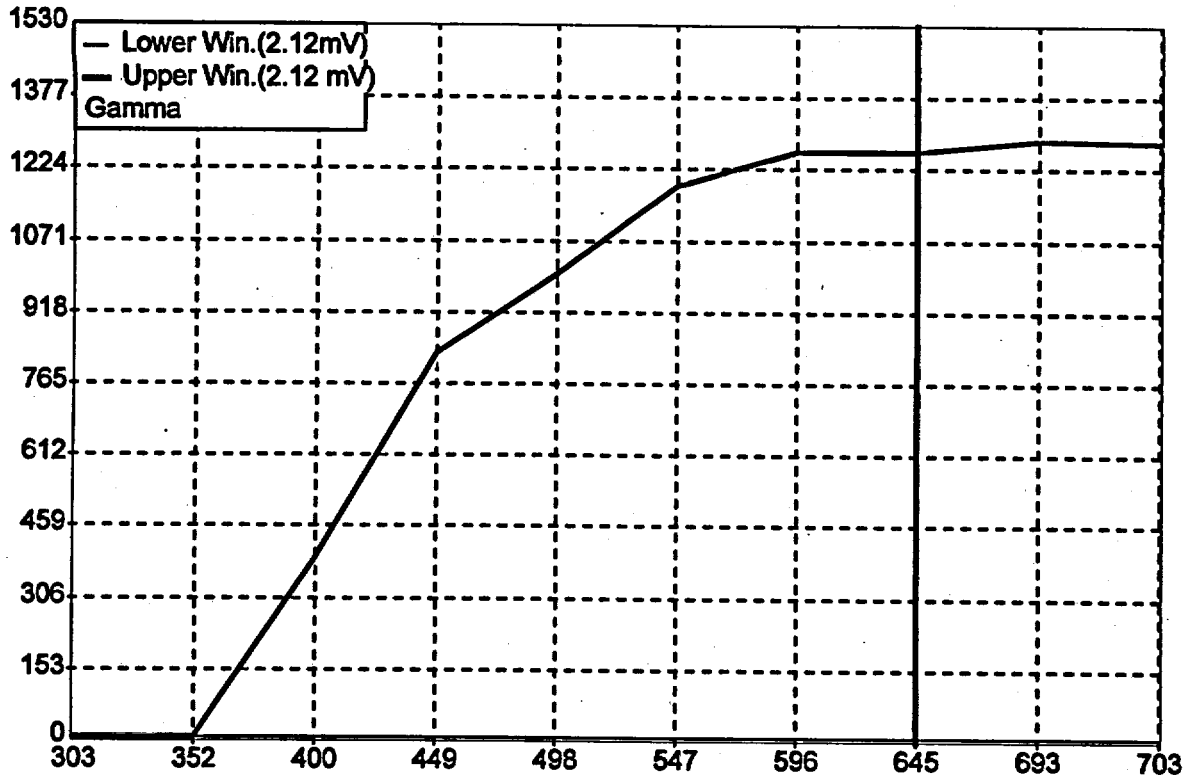

645:	0.00
	1254.13

Voltage

EBERLINE SPA-8 CALIBRATION REPORT

Date: 07/15/99
 Standard: Model 81
 SN: 7140

OUIC: W4GV91
 Isotope: Cs-137
 Type of Calibration: Source

E-600 Serial Number	921
Program Version	E600 V3.09
Calibration Date	12/30/98
Calibration Due Date	12/30/99
Scaler Precision	10%
Lower Threshold Slope	0.8718
Lower Threshold Intercept	-0.2205 mV
Upper Threshold Slope	0.9741
Upper Threshold Intercept	-0.6963 mV
Alarm Editing	Enabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	723412
Type	S-SPA-8
Calibration Date	07/15/99
Calibration Due Date	01/10/00
Dead Time	22.0 usec
Surface Area	5.00 cm ²
Max High Voltage	1500 Vdc
Overrange	45000 cps

Channel 1	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	576 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.16E+10 counts/R
Scaler Time	120 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 2	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	576 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.16E+10 counts/R
Scaler Time	120 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 3	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	576 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.16E+10 counts/R
Scaler Time	120 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0

Gamma Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
0.0040 R/hr	0.0041 R/hr	2.96%	Pass
0.0004 R/hr	0.0004 R/hr	6.85%	Pass
1.00E-04 R/hr	9.19E-05 R/hr	-8.10%	Pass
4.00E-05 R/hr	3.88E-05 R/hr	3.04%	Pass

Response Test Range: 8.92 - 13.38 μ R/hr (BKG CORRECTED)

Remarks:

This calibration is traceable to the National Institute of Standards and Technology.

Response tested with Cs-137, SN: CS-99R.


Performed By: Al Penella

Reviewed By: Cy Holly

Report number: 071599723412

SPA-8 723412 Voltage Plateau Curve

C
o
u
n
t
s
/
S
e
c

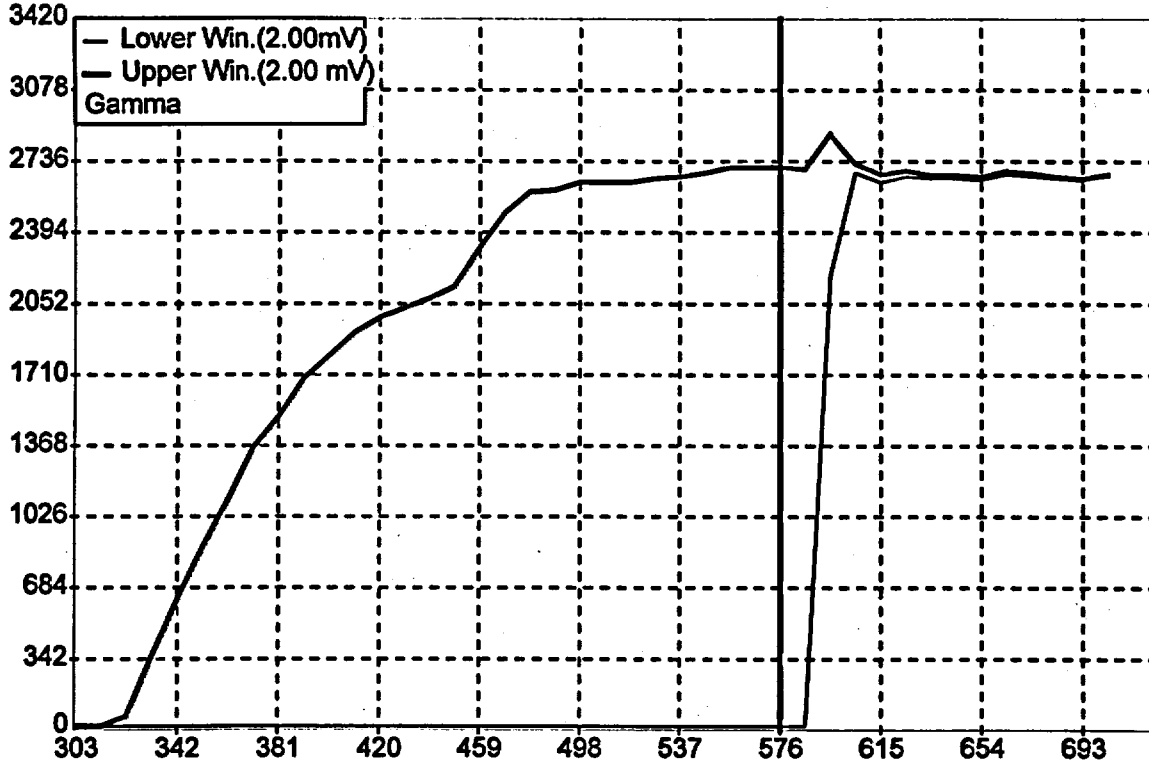

576:	0.00
	2692.59

Voltage

EBERLINE SPA-8 CALIBRATION REPORT

Date: 07/15/99
Standard: Model 81
SN: 7140

OUIC: W4GV91
Isotope: Cs-137
Type of Calibration: Source

E-600 Serial Number	921
Program Version	E600 V3.09
Calibration Date	12/30/98
Calibration Due Date	12/30/00
Scaler Precision	10%
Lower Threshold Slope	0.8718
Lower Threshold Intercept	-0.2205 mV
Upper Threshold Slope	0.9741
Upper Threshold Intercept	-0.6963 mV
Alarm Editing	Enabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	723415
Type	S-SPA-8
Calibration Date	07/15/99
Calibration Due Date	01/10/00
Dead Time	22.0 usec
Surface Area	5.00 cm ²
Max High Voltage	1500 Vdc
Overrange	45000 cps

Channel 1	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	596 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.18E+10 counts/R
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 2	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	596 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.00 counts/R
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 3	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	596 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.00 counts/R
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0

Gamma Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
0.0040 R/hr	0.0040 R/hr	1.07%	Pass
0.0004 R/hr	0.0004 R/hr	3.42%	Pass
1.00E-04 R/hr	9.06E-05 R/hr	-9.37%	Pass
4.00E-05 R/hr	3.98E-05 R/hr	0.5547%	Pass

Response Test Range: 8.13 - 12.20 μ R/hr (BKT CORRECTED)

Remarks:

This calibration is traceable to the National Institute of Standards and Technology.

Response tested with Cs-137, SN: CS-99R.


Performed By: Al Perrella

Reviewed By: Cj Holly

Report number: 071599723415

SPA-8 723415 Voltage Plateau Curve

C
o
u
n
t
s
/
S
e
c

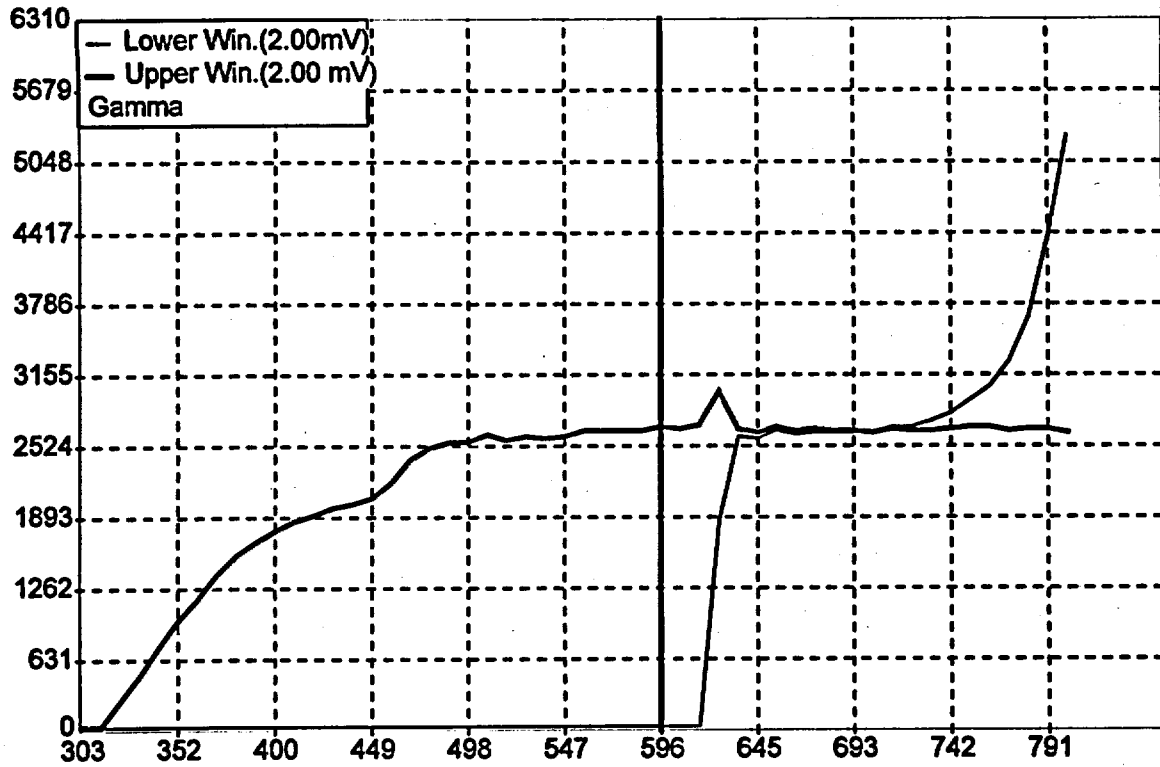

Voltage

EBERLINE SPA-8 CALIBRATION REPORT

Date: 05/11/99
Standard: Model 81
SN: 7140

OUIC: W4GV91
Isotope: Cs-137
Type of Calibration: Source

E-600 Serial Number	926
Program Version	E600 V3.09
Calibration Date	01/01/99
Calibration Due Date	12/30/99
Scaler Precision	10%
Lower Threshold Slope	0.9048
Lower Threshold Intercept	-0.0857 mV
Upper Threshold Slope	1.08
Upper Threshold Intercept	-0.5926 mV
Alarm Editing	Enabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	723416
Type	S-SPA-8
Calibration Date	05/11/99
Calibration Due Date	11/06/99
Dead Time	12.0 usec
Surface Area	5.00 cm ²
Max High Voltage	1500 Vdc
Overrange	45000 cps

Channel 1	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	10 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 2	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	10 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 3	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	10 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0

Gamma Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
0.0040 R/hr	0.0040 R/hr	3.17%	Pass
0.0004 R/hr	0.0004 R/hr	6.54%	Pass
1.00E-04 R/hr	9.81E-05 R/hr	-1.93%	Pass
4.00E-05 R/hr	3.90E-05 R/hr	-2.61%	Pass

Response Test Range: 11.24 - 16.86 μ R/hr (BKG CORRECTED)

Remarks:

This calibration is traceable to the National Institute of Standards and Technology.

Response tested with Cs-137, SN: CS-99R. As found data within specifications. No high voltage plateau performed.

Date of next calibration: 6 NOV 99.

Performed By: Al Penelle

Reviewed By: Bob [Signature]

Report number: 051199723416

EBERLINE SPA-8 CALIBRATION REPORT

Date: 05/11/99
Standard: Model 81
SN: 7140

OUI: W4GV91
Isotope: Cs-137
Type of Calibration: Source

E-600 Serial Number	951
Program Version	E600 V3.09
Calibration Date	12/01/98
Calibration Due Date	12/30/99
Scaler Precision	10%
Lower Threshold Slope	0.8205
Lower Threshold Intercept	-0.1487 mV
Upper Threshold Slope	0.9741
Upper Threshold Intercept	-0.6963 mV
Alarm Editing	Disabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	724038
Type	SSPA-8
Calibration Date	05/11/99
Calibration Due Date	11/06/99
Dead Time	15.5 usec
Surface Area	5.00 cm ²
Max High Voltage	1500 Vdc
Overrange	45000 cps

Channel 1	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	645 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.06E+10 counts/R
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 2	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	645 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.06E+10 counts/R
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 3	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	645 Vdc
Lower Threshold	2.12 mV
Upper Threshold	2.12 mV
Selected Window	Upper
Upper Cal. Constant	1.06E+10 counts/R
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0

Gamma Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
0.0040 R/hr	0.0044 R/hr	9.80%	Pass
0.0004 R/hr	0.0004 R/hr	8.73%	Pass
1.00E-04 R/hr	9.29E-05 R/hr	-7.14%	Pass
4.00E-05 R/hr	3.95E-05 R/hr	-1.17%	Pass

Response Test Range: 7.13 - 10.69 μ R/hr (BKT CORRECTED)

Remarks:

This calibration is traceable to the National Institute of Standards and Technology.

Response tested with Cs-137, SN: CS-99R. As found data within specifications. No high voltage plateau performed.

Date of next calibration: 6 NOV 99.

Performed By: W Perrella

Reviewed By: Durt Hummer

Report number: 051199724038

EBERLINE SPA-8 CALIBRATION REPORT

Date: 05/11/99
Standard: Model 81
SN: 7140

OUI: W4GV91
Isotope: Cs-137
Type of Calibration: Source

E-600 Serial Number	1358
Program Version	E600 V3.09
Calibration Date	12/31/98
Calibration Due Date	12/31/99
Scaler Precision	10%
Lower Threshold Slope	0.8810
Lower Threshold Intercept	-0.1905 mV
Upper Threshold Slope	0.9222
Upper Threshold Intercept	-0.8889 mV
Alarm Editing	Enabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	723413
Type	S-SPA-8
Calibration Date	05/11/99
Calibration Due Date	11/06/99
Dead Time	18.0 usec
Surface Area	5.00 cm ²
Max High Voltage	1500 Vdc
Overrange	45000 cps

Channel 1	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	120 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 2	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	120 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0
Channel 3	
Channel Type	Gamma
Rate Units	R/hr
Response Times	20,10,3 secs
High Voltage	693 Vdc
Lower Threshold	2.00 mV
Upper Threshold	2.00 mV
Selected Window	Upper
Upper Cal. Constant	1.00E+10 counts/R
Scaler Time	120 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.0

Gamma Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
0.0040 R/hr	0.0042 R/hr	6.24%	Pass
0.0004 R/hr	0.0004 R/hr	7.07%	Pass
1.00E-04 R/hr	9.28E-05 R/hr	-7.19%	Pass
4.00E-05 R/hr	4.07E-05 R/hr	1.74%	Pass

Response Test Range: 11.84 - 17.76 μ R/hr (BKG CORRECTED)

Remarks:

This calibration is traceable to the National Institute of Standards and Technology.

Response tested with Cs-137, SN: CS-99R. As found data within specifications. No high voltage plateau performed.

Date of next calibration: 6 NOV 99.

Performed By: Al Perrella

Reviewed By: Burt Hummer

Report number: 051199723413

EBERLINE SHP-380AB CALIBRATION REPORT

Date: 03/01/99 Detector SN: 579 Detector Type: Scintillation
 Type of Calibration: Source OJIC: W4GV91

Standards:

Isotope: Pu-239 Model: AN/UDM-6 Serial Number: A0026
 Isotope: Tc-99 Model: DNS-19 Serial Number: TC-01

E-600 Serial Number	921
Program Version	E600 V3.09
Calibration Date	12/30/97
Calibration Due Date	12/30/99
Scaler Precision	10%
Lower Threshold Slope	0.8718
Lower Threshold Intercept	-0.2205 mV
Upper Threshold Slope	0.9741
Upper Threshold Intercept	-0.6963 mV
Alarm Editing	Enabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	579
Type	SHP380AB
Calibration Date	03/01/99
Calibration Due Date	08/27/99
Dead Time	8.00 usec
Surface Area	100 cm ²
Max High Voltage	1000 Vdc
Overrange	80000 cps

Channel 1	
Channel Type	Alpha
Rate Units	cpm
Response Times	20,20,20 secs
High Voltage	703 Vdc
Lower Threshold	1.50 mV
Upper Threshold	30.1 mV
Selected Window	Upper
Upper Cal. Constant	1.00 counts/count
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.2323
Channel 2	
Channel Type	Beta
Rate Units	cpm
Response Times	20,20,20 secs
High Voltage	703 Vdc
Lower Threshold	1.50 mV
Upper Threshold	30.1 mV
Selected Window	Lower
Lower Cal. Constant	1.00 counts/count
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.2323
Channel 3	
Channel Type	Alpha/Beta
Rate Units	cpm
Response Times	20,20,20 secs
High Voltage	703 Vdc
Lower Threshold	1.50 mV
Upper Threshold	30.1 mV
Selected Window	Both
Lower Cal. Constant	1.00 counts/count
Upper Cal. Constant	1.00 counts/count
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.2323

Alpha Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
1.76E+05 cpm	1.73E+05 cpm	-1.79%	Pass
16361 cpm	17018 cpm	4.02%	Pass
1206 cpm	1146 cpm	-4.98%	Pass

Beta Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
1.13E+05 cpm	1.06E+05 cpm	-6.49%	Pass
10516 cpm	10103 cpm	-3.92%	Pass
2316 cpm	2218 cpm	-4.24%	Pass
1586 cpm	1493 cpm	-5.89%	Pass

EFFICIENCY: ALPHA: 28.93% BETA: 15.31%

Remarks:

This Calibration is Traceable to the National Institute of Standards and Technology.
Background values added to source activity for linearity test.
Background values: Alpha: 17 cpm Beta: 1476 cpm


Date of next calibration: 27 AUG 1999

Performed By: Al Perrella

Reviewed By: Burt Lanning

Report Number: 030199579

SHP 380AB SN: 579 Voltage Plateau Curve

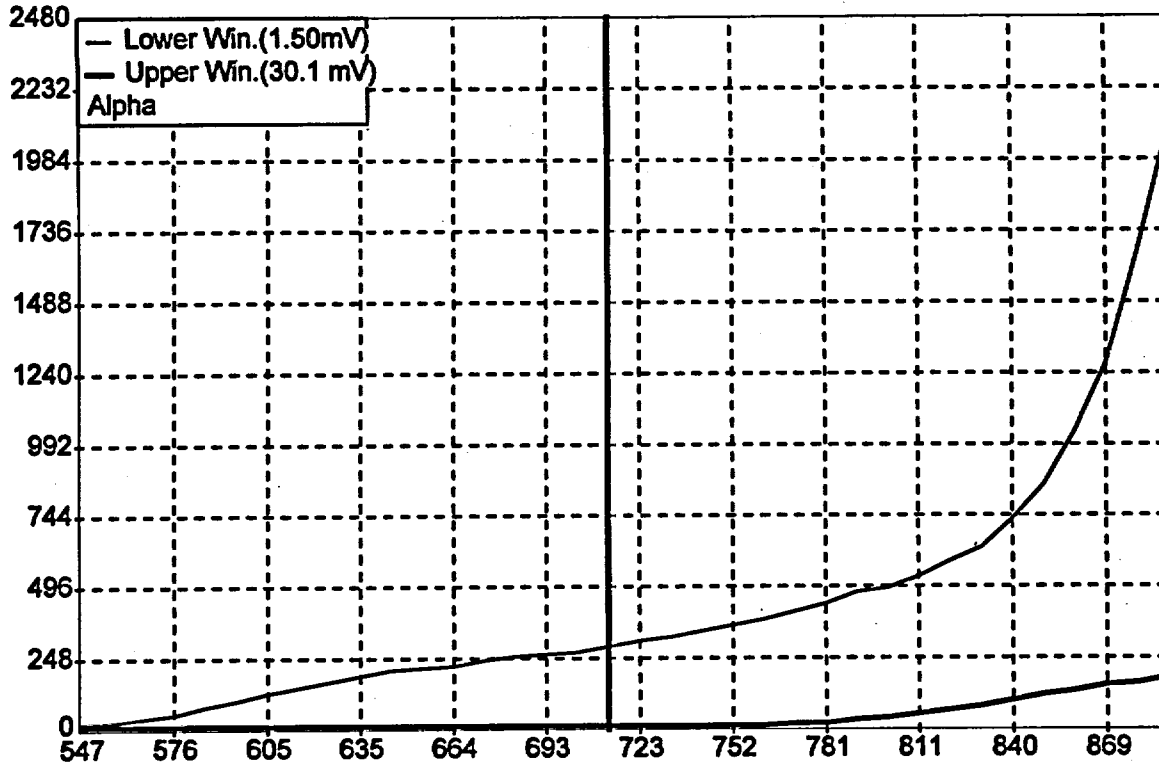

C
o
u
n
t
s
/
S
e
c

713:	276.63
	0.10

Voltage

EBERLINE SHP-380AB CALIBRATION REPORT

Date: 02/26/99 Detector SN: 179 Detector Type: Scintillation
 Type of Calibration: Source OUIIC: W4GV91

Standards:

Isotope: Pu-239 Model: AN/UDM-6 Serial Number: A0026
 Isotope: Tc-99 Model: DNS-19 Serial Number: TC-01

E-600 Serial Number	921
Program Version	E600 V3.09
Calibration Date	12/30/97
Calibration Due Date	12/30/99
Scaler Precision	10%
Lower Threshold Slope	0.8718
Lower Threshold Intercept	-0.2205 mV
Upper Threshold Slope	0.9741
Upper Threshold Intercept	-0.6963 mV
Alarm Editing	Enabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	179
Type	SHP380
Calibration Date	02/26/99
Calibration Due Date	08/24/99
Dead Time	8.00 usec
Surface Area	100 cm ²
Max High Voltage	1000 Vdc
Overrange	80000 cps

Channel 1	
Channel Type	Alpha
Rate Units	cpm
Response Times	20,20,20 secs
High Voltage	732 Vdc
Lower Threshold	1.50 mV
Upper Threshold	30.1 mV
Selected Window	Upper
Upper Cal. Constant	1.00 counts/count
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.2237
Channel 2	
Channel Type	Beta
Rate Units	cpm
Response Times	20,20,20 secs
High Voltage	732 Vdc
Lower Threshold	1.50 mV
Upper Threshold	30.1 mV
Selected Window	Lower
Lower Cal. Constant	1.00 counts/count
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.2237
Channel 3	
Channel Type	Alpha/Beta
Rate Units	cpm
Response Times	20,20,20 secs
High Voltage	732 Vdc
Lower Threshold	1.50 mV
Upper Threshold	30.1 mV
Selected Window	Both
Lower Cal. Constant	1.00 counts/count
Upper Cal. Constant	1.00 counts/count
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.2237

Alpha Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
1.76E+05 cpm	1.68E+05 cpm	-4.42%	Pass
16358 cpm	15661 cpm	-4.26%	Pass
1203 cpm	1119 cpm	-7.01%	Pass

Beta Channel Linearity Test Results - Pass Tolerance Plus/Minus 10.0%

Field	Response	%Error	Pass/Fail
1.14E+05 cpm	1.09E+05 cpm	-4.07%	Pass
10560 cpm	9698 cpm	-8.16%	Pass
2360 cpm	2161 cpm	-8.42%	Pass
1630 cpm	1648 cpm	1.08%	Pass

EFFICIENCY: ALPHA: 22.37% BETA: 16.45%

Remarks:

This Calibration is Traceable to the National Institute of Standards and Technology.
Background values added to source activity for linearity test.
Background values: Alpha: 14 cpm Beta: 1520 cpm

Date of next calibration: 24 AUG 1999


Performed By: Al Perrella

Reviewed By: Bush Cummings

Report Number: 022699179

SHP 380AB SN: 179 Voltage Plateau Curve

C
o
u
n
t
s
/
S
e
c

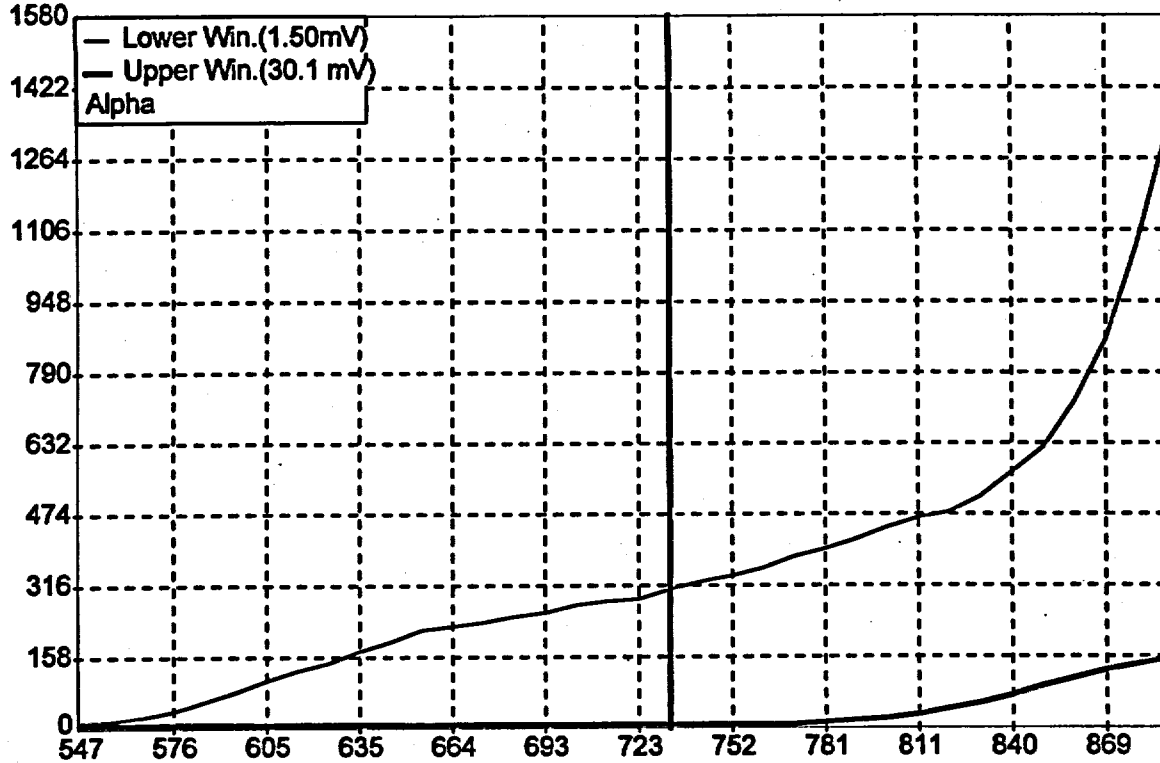

732:	299.38
	0.00

Voltage

EBERLINE SHP-380AB CALIBRATION REPORT

Date: 02/26/99

Detector SN: 605

Detector Type: Scintillation

Type of Calibration: Source OUIIC: W4GV91

Standards:

Isotope: Pu-239

Model: AN/UDM-6

Serial Number: A0026

Isotope: Tc-99

Model: DNS-19


Serial Number: TC-01

E-600 Serial Number	921
Program Version	E600 V3.09
Calibration Date	12/30/97
Calibration Due Date	12/30/99
Scaler Precision	10%
Lower Threshold Slope	0.8718
Lower Threshold Intercept	-0.2205 mV
Upper Threshold Slope	0.9741
Upper Threshold Intercept	-0.6963 mV
Alarm Editing	Enabled
Latching Alarms	Disabled
Auto Ranging	Enabled
Beep on Auto-Range	No
Ignore E-600 Cal. Date	Yes
Ignore Probe Cal. Date	No
Ratemeter Mode Support	Enabled
Integrate Mode Support	Disabled
Scaler Mode Support	Enabled
Peak Hold Mode Support	Disabled
Background Update Mode Support	Disabled
Log ID Source	Internal/Aux.
Star Key Ratemeter Function	Zero Display
Star Key Integrate Function	Zero Display
Scaler Display Units	Dose
Scaler Counting Mode	Fixed Time
Smart Probe Serial Number	605
Type	SHP380
Calibration Date	02/26/99
Calibration Due Date	08/24/99
Dead Time	8.00 usec
Surface Area	100 cm ²
Max High Voltage	1000 Vdc
Overrange	80000 cps

Channel 1	
Channel Type	Alpha
Rate Units	cpm
Response Times	20,20,20 secs
High Voltage	771 Vdc
Lower Threshold	1.50 mV
Upper Threshold	30.1 mV
Selected Window	Upper
Upper Cal. Constant	1.00 counts/count
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.2809
Channel 2	
Channel Type	Beta
Rate Units	cpm
Response Times	20,20,20 secs
High Voltage	771 Vdc
Lower Threshold	1.50 mV
Upper Threshold	30.1 mV
Selected Window	Lower
Lower Cal. Constant	1.00 counts/count
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.2809
Channel 3	
Channel Type	Alpha/Beta
Rate Units	cpm
Response Times	20,20,20 secs
High Voltage	771 Vdc
Lower Threshold	1.50 mV
Upper Threshold	30.1 mV
Selected Window	Both
Lower Cal. Constant	1.00 counts/count
Upper Cal. Constant	1.00 counts/count
Scaler Time	60 secs
Lower to Upper Crossover	0.0
Upper to Lower Crossover	0.2809

SHP 380AB SN: 605 Voltage Plateau Curve

C
o
u
n
t
s
/
S
e
c

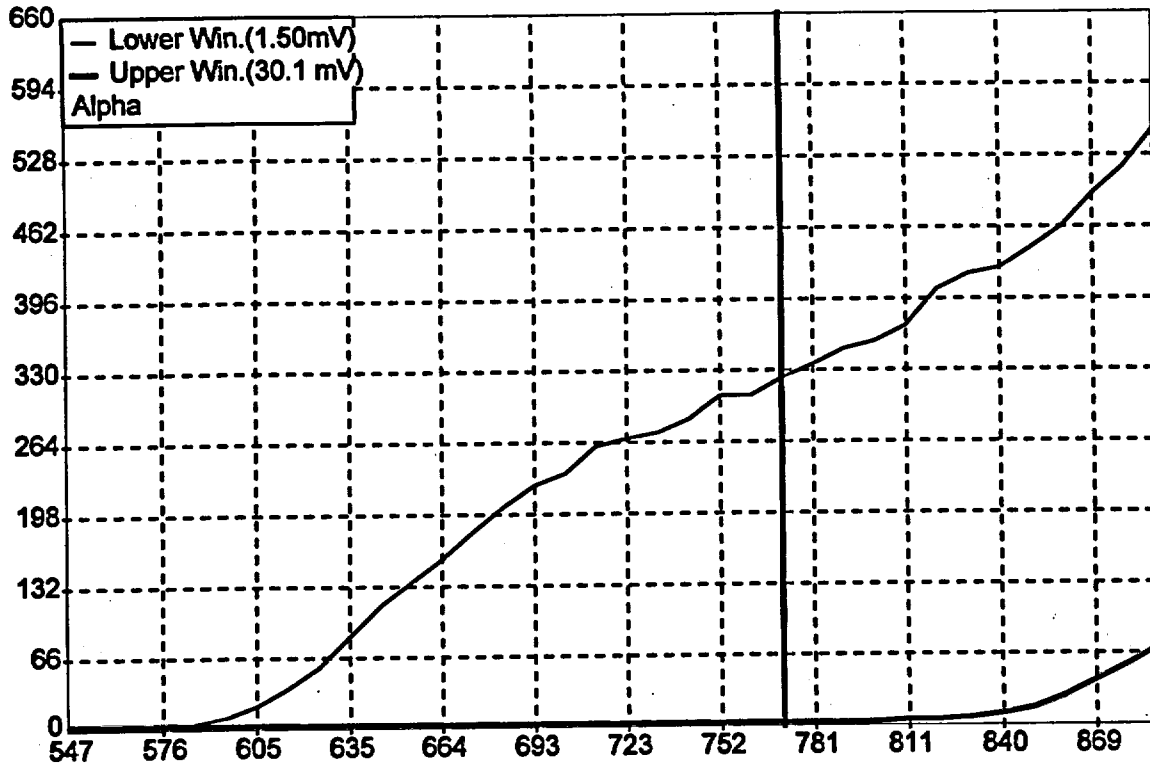

771:	319.29
	0.00

Voltage

Soil 9006

Grid Number	Gross Alpha	Net Alpha	Gross Beta	Net Beta	Gross Gamma	Net Gamma	Alpha	Beta	Gamma
	pCi/gm	pCi/gm	pCi/gm	pCi/gm	pCi/gm	pCi/gm			
S01	2.908	0.307	6.857	1.416	5.314	-2.852	2.601	5.241	8.166
S02	2.991	0.390	6.316	1.075	4.574	-3.592			
S03	1.491	-1.110	3.403	-1.838	3.737	-4.429			
S04	2.595	-0.006	4.459	-0.782	4.936	-3.230			
S05	1.918	-0.683	2.295	-2.946	9.037	0.871			
S06	2.051	-0.550	3.475	-1.766	3.770	-4.396			
S07	1.340	-1.261	2.466	-2.775	5.957	-2.209			
S08	1.960	-0.641	4.317	-0.924	7.813	-0.353			
S09	2.185	-0.416	4.440	-0.801	8.530	0.364			
S10	1.036	-1.565	2.046	-3.195	8.341	0.175			

Soil 9010

Grid Number	Gross Alpha	Net Alpha	Gross Beta	Net Beta	Gross Gamma	Net Gamma	Alpha	Beta	Gamma
	pCi/gm	pCi/gm	pCi/gm	pCi/gm	pCi/gm	pCi/gm			
S01	2.240	-0.361	4.158	-1.083	3.259	-4.907	2.601	5.241	8.166
S02	2.640	0.039	7.105	1.864	7.985	-0.181			
S03	1.243	-1.358	4.304	-0.937	5.312	-2.854			
S04	1.884	-0.717	3.315	-1.926	4.968	-3.198			
S05	1.879	-0.722	5.543	0.302	6.420	-1.746			
S06	1.407	-1.194	2.571	-2.670	4.011	-4.155			
S07	2.274	-0.327	8.446	3.205	9.205	1.039			
S08	2.429	-0.172	4.384	-0.857	5.158	-3.008			
S09	1.990	-0.611	2.001	-3.240	6.062	-2.104			
S10	2.736	0.135	4.410	-0.831	8.060	-0.106			
S11	1.420	-1.181	6.253	1.012	7.470	-0.696			
S12	1.197	-1.404	2.665	-2.576	7.761	-0.405			
S13	1.244	-1.357	3.308	-1.933	7.121	-1.045			
S14	2.455	-0.146	2.406	-2.835	6.953	-1.213			
S15	1.503	-1.098	4.278	-0.963	5.415	-2.751			
S16	2.181	-0.420	5.649	0.408	6.701	-1.465			
S17	2.038	-0.563	15.226	9.985	7.459	-0.707			
S18	2.278	-0.323	2.659	-2.582	3.540	-4.626			
S19	3.836	1.235	9.851	4.610	6.552	-1.614			
S20	2.955	0.354	7.260	2.019	4.372	-3.794			

Enclosure 2

Encl 2

Contracts/Zone 3-4 data.xls

Soil 9010 (Cont'd)

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	Alpha	Beta	Gamma
S21	4.935	2.334	21.410	16.169	6.151	-2.015	2.601	5.241	8.166
S22	1.623	-0.978	2.707	-2.534	7.140	-1.026			
S23	5.895	3.294	16.316	11.075	6.675	-1.491			
S24	0.850	-1.751	8.807	3.666	6.390	-1.776			
S25	1.683	-0.918	2.630	-2.611	6.253	-1.913			
S26	2.786	0.185	6.243	1.002	6.799	-1.367			
S27	0.895	-1.706	2.775	-2.466	7.341	-0.825			
S28	1.966	-0.635	9.145	3.904	5.056	-3.110			
S29	1.606	-0.995	2.790	-2.451	7.656	-0.510			
S30	0.625	-1.976	1.701	-3.540	7.630	-0.536			
S17E	2.515	-0.086	2.139	-3.102	7.503	-0.663			
S17N	3.976	1.375	4.091	-1.150	7.708	-0.458			
S17R	3.489	0.888	3.324	-1.917	6.845	-1.321			
S17S	2.941	0.340	2.497	-2.744	7.092	-1.074			
S17W	2.787	0.186	4.659	-0.582	6.910	-1.256			
S20E	1.288	-1.313	0.542	-4.699	4.407	-3.759			
S20N	1.290	-1.311	1.534	-3.707	4.441	-3.725			
S20R	1.899	-0.702	2.996	-2.245	3.186	-4.980			
S20S	0.930	-1.671	0.599	-4.642	3.644	-4.522			
S20W	1.839	-0.762	1.903	-3.338	3.127	-5.039			
S21E	2.709	0.108	2.946	-2.295	6.812	-1.354			
S21N	1.509	-1.092	1.566	-3.675	7.056	-1.110			
S21R	0.523	-2.078	1.150	-4.091	6.618	-1.548			
S21S	0.910	-1.691	3.133	-2.108	7.328	-0.840			
S21W	1.310	-1.291	3.005	-2.236	5.679	-2.487			
S23E	3.953	1.352	5.361	0.120	9.691	1.525			
S23N	3.746	1.145	3.865	-1.376	9.052	0.886			
S23R	3.992	1.391	3.781	-1.460	9.280	1.114			
S23S	4.282	1.681	4.182	-1.059	1.033	-7.133			
S23W	2.272	-0.329	2.995	-2.246	8.669	0.703			

Soil 9011

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S01	3.420	0.819	3.557	-1.684	7.469	-0.697	2.601	5.241	8.166
S02	0.419	-2.182	3.078	-2.163	6.720	-1.446			
S03	2.448	-0.153	2.789	-2.452	5.986	-2.180			
S04	2.773	0.172	7.640	2.399	8.528	0.362			
S05	2.398	-0.203	3.265	-1.976	4.438	-3.728			
S06	2.191	-0.410	3.909	-1.332	7.921	-0.245			
S07	4.219	1.618	5.080	-0.161	5.160	-3.006			
S08	1.469	-1.132	4.892	-0.349	6.284	-1.882			
S09	1.795	-0.806	2.653	-2.588	6.005	-2.161			
S10	2.665	0.064	2.730	-2.511	4.721	-3.445			

Soil 9011A

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S01	2.531	-0.070	10.809	5.568	8.499	0.333	2.601	5.241	8.166
S02	6.203	3.602	23.318	18.077	7.670	-0.496			
S03	5.759	3.158	22.648	17.407	7.397	-0.769			
S04	2.862	0.261	2.878	-2.363	7.657	-0.509			
S05	4.703	2.102	17.367	12.126	9.929	1.763			
S06	1.246	-1.355	2.309	-2.932	7.093	-1.073			
S07	2.058	-0.543	4.287	-0.954	6.191	-1.975			
S08	3.269	0.668	3.751	-1.490	1.001	-7.165			
S09	0.457	-2.144	3.025	-2.216	9.885	1.719			
S10	1.910	-0.691	5.578	0.337	7.912	-0.254			
S11	3.069	0.468	7.274	2.033	9.262	1.096			
S12	2.586	-0.015	7.238	1.997	5.829	-2.337			
S13	3.617	1.016	9.182	3.941	9.857	1.691			

Soil 9032

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S01	1.471	-1.130	4.561	-0.680	6.920	-1.246	2.601	5.241	8.166
S02	1.474	-1.127	3.840	-1.401	8.523	0.357			
S03	3.011	0.410	5.695	0.454	7.413	-0.753			
S04	1.971	-0.630	3.679	-1.562	5.674	-2.492			
S05	2.885	0.284	2.644	-2.597	6.420	-1.746			
S06	1.019	-1.582	3.313	-1.928	5.317	-2.849			
S07	2.355	-0.246	1.921	-3.320	6.637	-1.529			
S08	2.109	-0.492	3.291	-1.950	8.485	0.319			
S09	1.387	-1.214	3.176	-2.065	6.134	-2.032			
S10	2.253	-0.348	3.882	-1.359	5.804	-2.362			
S11	2.594	-0.007	4.074	-1.167	7.464	-0.702			
S12	0.971	-1.630	3.086	-2.155	6.148	-2.018			
S13	1.435	-1.166	2.667	-2.574	7.163	-1.003			
S14	1.125	-1.476	3.585	-1.656	8.225	0.059			
S15	1.774	-0.827	3.561	-1.680	6.229	-1.937			
S16	2.527	-0.074	10.703	5.462	7.237	-0.929			
S17	2.372	-0.229	8.270	3.029	1.266	-6.900			
S18	0.948	-1.653	3.907	-1.334	5.552	-2.614			
S19	2.085	-0.516	3.340	-1.901	8.293	0.127			
S20	1.325	-1.276	3.903	-1.338	8.863	0.697			
S21	2.022	-0.579	6.066	0.825	9.289	1.123			
S22	1.947	-0.654	3.874	-1.367	6.094	-2.072			
S23	0.501	-2.100	2.949	-2.292	5.386	-2.780			
S24	1.809	-0.792	4.076	-1.165	7.478	-0.688			
S25	1.432	-1.169	2.902	-2.339	6.509	-1.657			
S26	3.114	0.513	6.172	0.931	1.664	-6.502			
S27	2.068	-0.533	2.727	-2.514	5.886	-2.480			
S28	1.656	-0.945	4.362	-0.879	6.424	-1.742			
S29	1.959	-0.642	3.644	-1.597	7.399	-0.767			
S30	0.888	-1.713	2.320	-2.921	6.016	-2.150			
S31	0.766	-1.835	2.632	-2.609	7.807	-0.359			
S32	1.468	-1.133	1.957	-3.284	6.323	-1.843			
S33	0.947	-1.654	4.262	-0.979	9.949	1.783			
S34	1.444	-1.157	3.248	-1.993	1.424	-6.742			

Soil 9036

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	Alpha 2.601	Beta 5.241	Gamma 8.166
S01	3.647	1.046	21.844	16.603	6.861	-1.305			
S02	0.067	-2.534	6.254	1.013	5.878	-2.288			
S03	3.798	1.197	6.458	1.217	9.271	1.105			
S04	2.110	-0.491	8.377	3.136	9.400	1.234			
S05	2.783	0.182	10.122	4.881	1.057	-7.109			
S06	5.467	2.866	21.786	16.545	8.478	0.312			
S07	2.756	0.155	7.591	2.350	7.184	-0.982			
S08	3.913	1.312	4.556	-0.685	1.134	-7.032			
S09	4.488	1.887	6.504	1.263	1.160	-7.006			
S10	1.235	-1.366	6.785	1.544	1.218	-6.948			
S11	2.570	-0.031	5.573	0.332	5.665	-2.601			
S12	2.081	-0.520	5.328	0.087	8.852	0.686			
S13	2.110	-0.491	3.032	-2.209	7.159	-1.007			
S14	3.637	1.036	21.253	16.012	1.550	-6.616			
S15	5.578	2.977	18.480	13.239	4.104	-4.062			
S16	2.416	-0.185	6.811	1.570	7.400	-0.766			
S17	2.733	0.132	8.057	2.816	7.020	-1.146			
S18	2.576	-0.025	5.589	0.348	2.305	-5.861			
S19	2.984	0.383	4.544	-0.697	7.460	-0.706			
S20	3.969	1.368	12.730	7.489	1.048	-7.118			
S21	1.932	-0.669	7.977	2.736	8.924	0.758			
S22	2.329	-0.272	7.833	2.592	1.077	-7.089			
S23	2.227	-0.374	4.551	-0.690	1.091	-7.075			
S24	7.250	4.649	15.700	10.459	6.958	-1.208			
S25	2.452	-0.149	2.770	-2.471	7.807	-0.359			
S26	0.735	-1.866	2.480	-2.761	1.014	-7.162			
S27	1.780	-0.821	5.099	-0.142	1.046	-7.120			
S28	2.774	0.173	2.784	-2.457	8.098	-0.068			
S01E	2.222	-0.379	2.309	-2.932	6.225	-1.941			
S01N	1.895	-0.706	2.111	-3.130	6.270	-1.896			
S01R	1.412	-1.189	2.588	-2.653	5.753	-2.413			
S01S	1.940	-0.661	4.902	-0.339	7.090	-1.076			
S01W	2.554	-0.047	4.203	-1.038	6.433	-1.733			
S05E	1.485	-1.116	1.531	-3.710	7.532	-0.634			
S05N	1.995	-0.606	2.367	-2.874	8.246	0.080			
S05R	3.712	1.111	5.628	0.387	6.812	-1.354			

Soil 9036 (Cont'd)

Grid Number	Gross Alpha	Net Alpha	Gross Beta	Net Beta	Gross Gamma	Net Gamma	Alpha	Beta	Gamma
	pCi/gm	pCi/gm	pCi/gm	pCi/gm	pCi/gm	pCi/gm			
S05S	1.747	-0.854	1.107	-4.134	5.672	-2.494	2.601	5.241	8.166
S05W	2.971	0.370	3.774	-1.467	7.154	-1.012			
S06R	1.619	-0.982	1.746	-3.495	7.472	-0.694			
S06W	1.780	-0.821	2.122	-3.119	6.257	-1.909			
S14E	6.837	4.236	7.092	1.851	7.996	-0.170			
S14N	1.685	-0.916	4.366	-0.875	7.153	-1.013			
S14R	2.999	0.398	4.565	-0.676	6.925	-1.241			
S14S	4.634	2.033	6.157	0.916	8.397	0.231			
S14W	8.481	5.880	15.294	10.053	9.160	0.994			
S15E	6.797	4.196	5.417	0.176	8.691	0.525			
S15N	4.331	1.730	9.390	4.149	8.956	0.790			
S15R	8.523	5.922	7.067	1.826	8.226	0.060			
S15S	2.249	-0.352	6.014	0.773	8.525	0.359			
S15W	10.055	7.454	9.678	4.437	7.645	-0.521			
S20E	8.317	5.716	9.764	4.523	1.203	-6.963			
S20N	4.902	2.301	6.022	0.781	7.536	-0.630			
S20R	7.095	4.494	6.120	0.879	8.748	0.582			
S20S	7.319	4.718	7.467	2.226	1.066	-7.100			
S20W	4.416	1.815	4.615	-0.626	7.197	-0.969			
S24E	5.988	3.387	7.968	2.727	8.599	0.433			
S24N	3.947	1.346	3.724	-1.517	8.160	-0.006			
S24R	5.794	3.193	6.319	1.078	7.369	-0.797			
S24S	7.760	5.159	4.896	-0.345	9.260	1.094			
S24W	6.714	4.113	6.136	0.895	8.842	0.676			

Soil 9037

Grid Number	Gross Alpha	Net Alpha	Gross Beta	Net Beta	Gross Gamma	Net Gamma	Alpha	Beta	Gamma
	pCi/gm	pCi/gm	pCi/gm	pCi/gm	pCi/gm	pCi/gm			
S01	2.528	-0.073	11.155	5.914	8.467	0.301	2.601	5.241	8.166
S02	4.592	1.991	17.958	12.717	9.960	1.794			
S03	5.752	3.151	19.167	13.926	6.685	-1.481			
S04	3.717	1.116	8.766	3.525	7.005	-1.161			
S05	3.197	0.596	4.567	-0.674	5.517	-2.649			
S06	3.321	0.720	14.475	9.234	6.040	-2.126			

Soil 9037 (Cont'd)

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	Alpha	Beta	Gamma
							2.601	5.241	8.166
S07	1.537	-1.064	3.440	-1.801	8.311	0.145			
S08	2.081	-0.520	8.458	3.217	7.648	-0.618			
S09	4.013	1.412	9.101	3.860	1.163	-7.003			
S10	3.350	0.749	8.687	3.446	6.344	-1.822			
S11	4.800	2.199	8.778	3.537	1.241	-6.925			
S12	4.552	1.951	5.457	0.216	9.258	1.092			
S13	4.229	1.628	8.192	2.951	8.987	0.821			
S14	2.504	-0.097	6.068	0.827	6.939	-1.227			
S15	3.069	0.468	4.839	-0.402	7.123	-1.043			
S16	1.981	-0.620	7.782	2.541	9.404	1.238			
S17	3.228	0.627	9.196	3.955	1.071	-7.095			
S18	2.439	-0.162	6.947	1.706	9.479	1.313			
S19	2.479	-0.122	5.213	-0.028	8.028	-0.140			
S20	2.491	-0.110	4.755	-0.486	6.350	-1.816			
S21	4.074	1.473	3.438	-1.803	8.304	0.138			
S22	7.681	5.080	28.732	23.491	4.305	-3.861			
S23	1.175	-1.426	4.680	-0.561	2.499	-5.667			
S24	2.293	-0.308	4.201	-1.040	7.241	-0.925			
S25	0.996	-1.605	4.731	-0.510	8.720	0.554			
S26	2.634	0.033	5.591	0.350	7.307	-0.859			
S27	1.530	-1.071	3.444	-1.797	8.964	0.798			
S28	1.738	-0.863	7.393	2.152	8.208	0.042			
S29	3.003	0.402	3.869	-1.372	7.618	-0.548			
S30	0.273	-2.328	3.420	-1.821	5.661	-2.505			

Soil 9037D

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	Alpha	Beta	Gamma
							2.601	5.241	8.166
S01	2.534	-0.067	3.713	-1.528	3.808	-4.358			
S02	1.922	-0.679	5.240	-0.001	6.126	-2.040			
S03	3.165	0.564	6.135	0.894	7.188	-0.978			
S04	2.406	-0.195	7.249	2.008	4.393	-3.773			
S05	3.045	0.444	4.308	-0.933	7.659	-0.507			
S06	2.393	-0.208	3.958	-1.283	6.961	-1.205			

Soil 9037D (Cont'd)

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S07	2.982	0.381	5.800	0.559	6.930	-1.236	2.601	5.241	8.166
S08	2.454	-0.147	5.474	0.233	7.759	-0.407			
S09	1.778	-0.823	5.919	0.678	7.793	-0.373			
S10	2.736	0.135	8.627	3.386	5.661	-2.505			
S11	1.223	-1.378	4.874	-0.367	4.119	-4.047			
S12	1.551	-1.050	3.695	-1.546	4.361	-3.805			
S13	2.518	-0.083	6.917	1.676	4.045	-4.121			
S14	2.456	-0.145	4.598	-0.643	3.925	-4.241			
S15	3.961	1.360	9.761	4.520	8.744	0.578			
S16	3.942	1.341	6.581	1.340	8.554	0.388			

Soil 9039

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S01	5.450	2.849	4.337	-0.904	7.426	-0.740	2.601	5.241	8.166
S02	4.018	1.417	4.035	-1.206	8.828	0.662			
S03	4.454	1.853	12.543	7.302	7.385	-0.781			
S04	2.460	-0.141	4.451	-0.790	7.841	-0.325			
S05	6.909	4.308	8.960	3.719	1.469	-6.697			
S06	2.319	-0.282	4.355	-0.886	6.085	-2.081			
S07	3.090	0.489	6.123	0.862	7.620	-0.546			
S08	4.294	1.693	12.454	7.213	1.216	-6.950			
S09	4.090	1.489	5.959	0.718	7.919	-0.247			
S10	2.683	0.082	4.246	-0.995	9.297	1.131			
S11	3.034	0.433	3.714	-1.527	8.031	-0.135			
S12	2.770	0.169	6.625	1.384	8.024	-0.142			
S13	2.884	0.283	2.948	-2.293	4.092	-4.074			
S14	1.250	-1.351	2.708	-2.533	4.869	-3.297			
S15	1.675	-0.926	2.153	-3.088	4.887	-3.279			
S16	1.805	-0.796	6.282	1.041	7.904	-0.262			
S17	1.959	-0.642	3.311	-1.930	6.223	-1.943			
S18	2.569	-0.032	2.480	-2.761	5.111	-3.055			
S19	1.666	-0.935	2.218	-3.023	4.064	-4.102			
S20	1.690	-0.911	1.741	-3.500	3.191	-4.975			

Soil 9039 (Cont'd)

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S21	1.986	-0.616	2.745	-2.496	5.936	-2.230	2.601	5.241	8.166
S22	2.141	-0.460	7.015	1.774	1.140	-7.026			
S23	4.535	1.934	6.429	1.188	6.453	-1.713			
S24	1.018	-1.583	1.591	-3.650	3.440	-4.726			
S25	2.516	-0.085	7.913	2.672	7.185	-0.981			
S26	1.464	-1.137	5.877	0.636	6.079	-2.087			
S27	1.794	-0.807	5.269	0.028	9.161	0.995			
S28	2.783	0.182	7.090	1.849	1.069	-7.097			
S29	5.339	2.738	7.076	1.835	1.063	-7.103			
S30	4.413	1.812	8.894	3.653	1.267	-6.899			
S31	2.041	-0.560	3.962	-1.279	1.062	-7.104			
S32	5.050	2.449	6.296	1.055	1.321	-6.845			

Soil 9040

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S01	1.961	-0.640	2.808	-2.433	8.446	0.280	2.601	5.241	8.166
S02	1.752	-0.849	2.328	-2.913	6.953	-1.213			
S03	2.385	-0.216	6.460	1.219	5.735	-2.431			
S04	1.903	-0.698	3.847	-1.394	5.914	-2.252			
S05	2.640	0.039	5.563	0.322	9.624	1.458			
S06	2.231	-0.370	4.375	-0.866	6.460	-1.706			
S07	1.255	-1.346	2.995	-2.246	6.579	-1.587			
S08	3.016	0.415	5.330	0.089	6.559	-1.607			
S09	1.993	-0.608	3.005	-2.236	8.781	0.615			
S10	2.674	0.073	3.433	-1.808	8.262	0.096			

Soil 9041

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	Alpha	Beta	Gamma
S01	4.253	1.652	8.167	2.926	9.917	1.761	2.601	5.241	8.166
S02	4.605	2.004	12.425	7.184	2.891	-5.275			
S03	5.209	2.608	6.496	1.255	5.092	-3.074			
S04	1.259	-1.342	4.807	-0.434	9.995	1.829			
S05	0.930	-1.671	4.764	-0.477	9.943	1.777			
S06	14.432	11.831	25.642	20.401	7.737	-0.429			
S07	3.909	1.308	11.597	6.356	1.137	-7.029			
S08	9.429	6.828	20.910	15.669	1.145	-7.021			
S09	9.288	6.687	19.320	14.079	1.121	-7.045			
S10	3.127	0.526	5.932	0.691	1.042	-7.124			

Soil 9047

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	Alpha	Beta	Gamma
S01	6.333	3.732	4.593	-0.648	7.811	-0.355	2.601	5.241	8.166
S02	4.218	1.617	4.760	-0.481	6.937	-1.229			
S03	4.107	1.506	7.061	1.820	1.096	-7.070			
S04	0.975	-1.626	4.397	-0.844	9.133	0.967			
S05	2.457	-0.144	4.022	-1.219	6.318	-1.848			
S06	1.198	-1.403	2.436	-2.805	2.111	-6.055			
S07	4.170	1.569	2.611	-2.630	9.440	1.274			
S08	4.008	1.407	4.383	-0.858	7.975	-0.191			
S09	2.751	0.150	4.022	-1.219	8.660	0.494			
S10	1.512	-1.089	2.569	-2.672	5.531	-2.635			
S11	4.664	2.063	7.737	2.496	1.375	-6.791			
S12	2.179	-0.422	2.504	-2.737	1.531	-6.635			

Soil 9049

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	Alpha	Beta	Gamma
S01	3.518	0.917	5.480	0.219	1.476	-6.690	2.601	5.241	8.166
S02	2.352	-0.249	3.157	-2.084	1.146	-7.020			
S03	2.641	0.040	4.792	-0.449	6.207	-1.959			
S04	2.023	-0.578	3.808	-1.433	4.141	-4.025			
S05	1.735	-0.866	2.436	-2.805	7.629	-0.537			
S06	3.244	0.643	6.424	1.183	1.204	-6.962			
S07	3.391	0.790	5.299	0.058	8.426	0.260			
S08	1.367	-1.234	4.911	-0.330	1.227	-6.939			
S09	3.615	1.014	4.809	-0.432	8.421	0.255			
S10	1.117	-1.484	4.032	-1.209	9.418	1.252			

Soil 9051

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	Alpha	Beta	Gamma
S01	2.737	0.136	3.434	-1.807	8.110	-0.056	2.601	5.241	8.166
S02	2.190	-0.411	3.704	-1.537	3.818	-4.348			
S03	3.767	1.166	6.446	1.205	7.378	-0.788			
S04	1.033	-1.568	4.178	-1.063	5.866	-2.300			
S05	2.554	-0.047	10.952	5.711	1.141	-7.025			
S06	2.683	0.082	5.028	-0.213	9.442	1.276			
S07	2.785	0.184	4.284	-0.957	9.699	1.533			
S08	3.715	1.114	7.511	2.270	6.419	-1.747			
S09	2.257	-0.344	4.353	-0.888	1.942	-6.224			
S10	1.373	-1.228	5.149	-0.092	1.854	-6.312			
S11	4.284	1.683	5.889	0.648	1.123	-7.043			
S12	2.563	-0.038	6.310	1.069	1.310	-6.856			
S13	2.979	0.378	5.949	0.708	1.207	-6.959			
S14	3.600	0.999	4.924	-0.317	8.519	0.353			
S15	1.579	-1.022	3.218	-2.023	6.536	-1.630			
S16	3.081	0.480	4.694	-0.547	6.850	-1.316			
S17	1.469	-1.132	3.735	-1.506	8.162	-0.004			

Soil 9053

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S01	3.074	0.473	4.028	-1.216	9.135	0.969	2.601	5.241	8.166
S02	3.578	0.977	6.932	1.691	1.081	-7.085			
S03	6.137	3.536	7.807	2.566	1.195	-6.971			
S04	3.345	0.744	6.814	1.573	9.129	0.963			
S05	2.224	-0.377	2.760	-2.481	5.947	-2.219			
S06	2.672	0.071	4.545	-0.696	1.251	-6.916			
S07	1.794	-0.807	3.734	-1.507	1.857	-6.309			
S08	3.151	0.550	4.576	-0.665	1.115	-7.051			
S09	1.786	-0.815	3.437	-1.804	7.462	-0.704			
S10	5.265	2.664	3.888	-1.353	7.722	-0.444			

Soil 9105

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S01	2.291	-0.310	3.456	-1.785	7.414	-0.752	2.601	5.241	8.166
S02	2.210	-0.391	3.168	-2.073	8.076	-0.090			
S03	2.718	0.117	4.340	-0.901	7.387	-0.779			
S04	1.329	-1.272	2.249	-2.992	7.444	-0.722			
S05	2.591	-0.010	5.261	0.020	7.366	-0.800			
S06	1.355	-1.246	1.702	-3.539	7.805	-0.361			
S07	3.217	0.616	1.887	-3.354	5.679	-2.487			
S08	2.217	-0.384	2.921	-2.320	7.782	-0.384			
S09	1.554	-1.047	4.607	-0.634	1.001	-7.165			
S10	1.124	-1.477	2.681	-2.560	9.363	1.197			

Soil 9400

<u>Grid Number</u>	<u>Gross Alpha pCi/gm</u>	<u>Net Alpha pCi/gm</u>	<u>Gross Beta pCi/gm</u>	<u>Net Beta pCi/gm</u>	<u>Gross Gamma pCi/gm</u>	<u>Net Gamma pCi/gm</u>	<u>Alpha</u>	<u>Beta</u>	<u>Gamma</u>
S01	2.916	0.315	5.454	0.213	9.000	0.834	2.601	5.241	8.166
S02	2.435	-0.166	4.997	-0.244	6.631	-1.535			
S03	3.355	0.754	4.744	-0.497	9.851	1.685			
S04	1.163	-1.438	4.167	-1.074	1.013	-7.153			
S05	1.618	-0.983	2.539	-2.702	7.928	-0.238			
S06	0.515	-2.086	4.100	-1.141	6.034	-2.132			
S07	4.755	2.154	3.919	-1.322	7.598	-0.568			
S08	2.371	-0.230	4.054	-1.187	6.452	-1.714			
S09	4.562	1.961	3.948	-1.293	6.813	-1.353			
S10	3.087	0.486	2.666	-2.575	7.182	-0.984			
S11	2.556	-0.045	4.412	-0.829	6.421	-1.745			
S12	2.032	-0.569	2.469	-2.772	6.753	-1.413			
S13	1.797	-0.804	2.422	-2.819	6.958	-1.208			
S14	1.047	-1.554	5.344	0.103	8.078	-0.088			
S15	1.392	-1.209	2.187	-3.054	7.745	-0.421			

September 22, 1999

Docket No. 030-05248
030-29741
Control No. 127060
127061

License No. 29-01022-06
29-01022-14

Joseph M. Santarsiero
Acting Director, Safety Risk Management
Department of the Army
U.S. Army Communications Electronics Command
AMSEL-SF-RER
Ft. Monmouth, NJ 07703-5024

Dear Mr. Santarsiero:

This is in reference to your letter dated July 14, 1999, requesting to amend Nuclear Regulatory Commission License Nos. 29-01022-06 and 29-01022-14. In order to continue our review, we need the following additional information:

1. Table 1 on page 11 in Section 2 provides your release criteria. Row 1 provides your tritium release criterion which is listed as 2000 disintegrations per minute (dpm)/ 100 cm² removable. The NRC criterion for release for unrestricted use for removable tritium is 1000 dpm/ 100 cm². Please provide a revised release criterion for tritium.
2. Surveys were not performed of the upper walls and ceilings of affected areas. NUREG/CR-5849 methodology would normally require surveys to be performed of the upper walls and ceilings of affected areas, however there are cases where surveys would not be required. Please provide either a detailed justification why surveys would not be required or the surveys.
3. Item 7 of Section 2 listed on page 15 lists the main parking lot as non-impacted. Past experience at numerous decommissioning sites has demonstrated that parking lots regularly can become contaminated at sites where radiological work has been performed over an extended period of time. Please provide your justification for classifying the parking lot as non-impacted or alternatively you could provide surveys of the parking lot.
4. Your submittal provides descriptions of the instruments used and the regular checks performed on them. It however, did not provide the calibration data for these instruments. Please provide the calibration data for the instruments used during your surveys. Also provide all the data on the instruments that were used for the scans.

ML10

5. NUREG/CR-5849 methodology requires reclassification of unaffected areas to affected areas if contamination in excess of 25 percent of the guideline value is identified. Numerous examples were identified during the NRC review of data points in excess of 25 percent of the guideline values were reported for unaffected areas. Some examples are Building 9011D R27, Building 9013 R13, Building 9393 R12, and Building 9043 R025. Please explain your reasoning for this apparent deviation from NUREG/CR-5849 methodology.
6. NUREG/CR-5849 methodology requires a minimum of 30 random sample points for unaffected survey units. A significant fraction of your unaffected survey units have less than 30 samples. Also, the survey units for open land areas are not clearly defined. As presented they appear to also not contain 30 samples per survey unit. Please explain your reasoning for this apparent deviation from NUREG/CR-5849 methodology.
7. The surveys of Building 9053 showed that there was some residual contamination in the sink in room 103. Were any surveys or scans taken of the sink trap for that sink? If so, please include them with your response to this letter.
8. All of the soil data provided in this submittal is in gross form. Please convert this data to net results so that they may be more easily compared with the release criteria.
9. Your September 10, 1999, letter roughly defines an area which is to be excluded from this release request. Please provide a detailed description of the area to be excluded from the release, including a diagram in your response would be very helpful.

We will continue our review upon receipt of this information. Please reply in duplicate to my attention at the Region I Office and refer to Mail Control Nos. 127060 and 127061. If you have any technical questions regarding this deficiency letter, please call me at (610) 337-5256.

If we do not receive a reply from you within 30 calendar days from the date of this letter, we shall assume that you do not wish to pursue your application.

Sincerely,

Original signed by Steven W. Shaffer

Steve W. Shaffer
Health Physicist
Decommissioning and Laboratory Branch
Division of Nuclear Materials Safety

Enclosures:
10 CFR Parts 19, 20, and 30
NUREG/CR-5849

J. Santarsiero
Department of the Army

3

DOCUMENT NAME: B:\DNMS Documents\Def Letter\29-1022-06.127060.wpd

1840371

To receive a copy of this document, indicate in the box: "C" = Copy w/o attach/encl "E" = Copy w/ attach/encl "N" = No copy

OFFICE	DNMS/RI	N	DNMS/RI				
NAME	SShaffer <i>SSW/S</i>						
DATE	09/22/99		09/ /99		09/ /99		09/ /99

OFFICIAL RECORD COPY



DEPARTMENT OF THE ARMY
HEADQUARTERS, US ARMY COMMUNICATIONS-ELECTRONICS COMMAND
AND FORT MONMOUTH
FORT MONMOUTH, NEW JERSEY 07703-5000

REPLY TO
ATTENTION OF

September 10, 1999

Directorate of Safety
Risk Management

U. S. Nuclear Regulatory Commission
Region 1
Attention: Mail Control #127060
(Mr. Steven Shaffer)
475 Allendale Road
King of Prussia, Pennsylvania 19406-1415

Dear Mr. Shaffer:

This refers to U.S. Nuclear Regulatory Commission (NRC) License Number 29-01022-06, Docket Number 030-05248, our letter of September 1, 1999, and to the September 8, 1999 telephone conversation between the undersigned and your Mr. Steven Shaffer.


To allow us to complete remediation efforts of the Zone 4A fenced compound, all Low Level Radioactive Waste (LLRW) will be moved onto Zone 4, on the asphalt area between the intersection of 6th Street and Avenues B and C. LLRW will be packaged in their shipping containers for ultimate disposal. We have submitted our amendment request to referenced NRC license, under separate cover, for authorization to temporary store LLRW at this location.

Based upon the above, we are requesting that you continue to review the Report, Radiological Status Survey of Buildings, Sewer System, and Soil in Survey Zone Three and Four at Evans Area, Fort Monmouth, New Jersey, provided to you on July 14, 1999.

We will address the aforementioned asphalt area, in an addendum to the above report, once the LLRW is shipped for disposal. The addendum to the report will follow shortly thereafter.

If we can provide you with anything further in this matter our point of contact is Mr. Richard Lovell, or the undersigned, on Voice (732) 427-4427/3112; or Facsimile (732) 532-6403 or (732) 542-7161.

Sincerely,

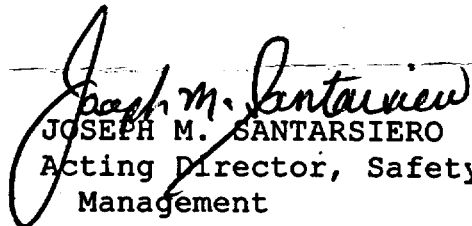
JOSEPH M. SANTARSIERO
Acting Director, Safety Risk
Management

Copy Furnished:

Commander, U.S. Army Materiel Command, ATTN: AMCSF-P,
5001 Eisenhower Avenue, Alexandria, Virginia 22333-0001



DEPARTMENT OF THE ARMY
HEADQUARTERS, US ARMY COMMUNICATIONS-ELECTRONICS COMMAND
AND FORT MONMOUTH
FORT MONMOUTH, NEW JERSEY 07703-5000

REPLY TO
ATTENTION OF

September 1, 1999

Directorate of Safety
Risk Management

U. S. Nuclear Regulatory Commission
Region 1
Attention: Mail Control #127060
(Mr. Steven Shaffer)
475 Allendale Road
King of Prussia, Pennsylvania 19406-1415

Dear Mr. Shaffer:

This refers to U.S. Nuclear Regulatory Commission (NRC) License Number 29-01022-06, Docket Number 030-05248, and to the August 23, 1999 telephone conversation between Messrs. Craig Miller and Steven A. Horne, IceSolv Inc., contracted to the Directorate of Safety Risk Management, and your Mr. Steven Shaffer.

We are in the process of requesting an amendment to the above NRC license to allow for the temporary storage of Low Level Radioactive Waste (LLRW) accumulated as a result of remediation efforts in support of the Base Realignment and Closure (BRAC) activities of the Evans Area. The LLRW accumulated, i.e., construction debris, is to be stored outside of the Zone 4A fenced compound, in order to allow us the ability to complete final status surveys of Zone 4A.

We propose to place all LLRW into Zone 4, on a grass-covered field on the Northwest corner at the intersection of Avenue B and 6th Street. All LLRW will be packaged in their shipping containers for ultimate disposal.

Based upon the above, we are requesting that you continue to review the Report, Radiological Status Survey of Buildings, Sewer System, and Soil in Survey Zone Three and Four at Evans Area, Fort Monmouth, New Jersey.

127060

SEP - 7 1999

Printed on  Recycled Paper


OFFICIAL RECORD COPY

ML 10

We will address the above field located on the Northwest of the intersection of 6th Street and Avenue B, Zone 4, in an addendum to the above report, once the LLRW is shipped to its final disposal site. The addendum to the report will follow shortly thereafter. Please note that this field was originally classified as Non-impacted, and thus was not surveyed or addressed in the above report.

If we can provide you with anything further in this matter our point of contact is Mr. Richard Lovell, or the undersigned, on Voice (732) 427-4427/3112; or Facsimile (732) 532-6403 or (732) 542-7161.

Sincerely,

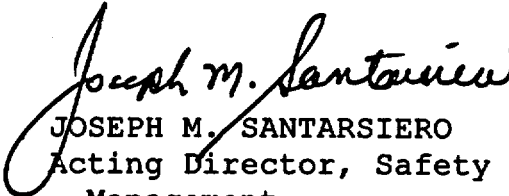
JOSEPH M. SANTARSIERO
Acting Director, Safety Risk
Management

Copy Furnished:

Commander, U.S. Army Materiel Command, ATTN: AMCSF-P,
5001 Eisenhower Avenue, Alexandria, Virginia 22333-0001

This is to acknowledge the receipt of your letter/application dated

7-14-99, and to inform you that the initial processing which includes an administrative review has been performed.

Amend. *29-01022-06*
There were no administrative omissions. Your application was assigned to a technical reviewer. Please note that the technical review may identify additional omissions or require additional information.

Please provide to this office within 30 days of your receipt of this card

A copy of your action has been forwarded to our License Fee & Accounts Receivable Branch, who will contact you separately if there is a fee issue involved.

Your action has been assigned Mail Control Number 127060.
When calling to inquire about this action, please refer to this control number.
You may call us on (610) 337-5398, or 337-5260.

MFC FORM 532 (R)
(8-88)

Sincerely,
Licensing Assistance Team Leader